

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081320\
 Data File : BF121273.D
 Acq On : 13 Aug 2020 16:30
 Operator : JU/CG
 Sample : PB130942BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130942BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	475	478	485	rBV	22485	26549	1.21%	0.204%
2	5.322	546	550	564	rBV	1594232	1437247	65.57%	11.048%
3	6.357	722	726	729	rBV	1652430	1377790	62.85%	10.591%
4	6.722	784	788	797	rVB	521828	437682	19.97%	3.364%
5	7.281	880	883	887	rBV	1088696	972424	44.36%	7.475%
6	8.004	1002	1006	1009	rBV	775814	580700	26.49%	4.464%
7	9.081	1185	1189	1192	rBV	2248316	1880184	85.77%	14.453%
8	9.751	1300	1303	1307	rBV	828061	667906	30.47%	5.134%
9	10.539	1433	1437	1449	rBV	1338202	1104581	50.39%	8.491%
10	11.233	1552	1555	1559	rBV	882844	715830	32.66%	5.503%
11	12.822	1821	1825	1828	rBV	2493804	2192080	100.00%	16.851%
12	13.868	1998	2003	2007	rBV	834885	727444	33.19%	5.592%
13	14.645	2125	2135	2141	rBV2	24764	44865	2.05%	0.345%
14	14.963	2185	2189	2192	rBV	25070	24616	1.12%	0.189%
15	15.286	2239	2244	2248	rBV	617514	686328	31.31%	5.276%
16	15.315	2248	2249	2255	rVB	26807	28567	1.30%	0.220%
17	15.727	2314	2319	2324	rBV	20553	31769	1.45%	0.244%
18	16.657	2472	2477	2484	rVB2	18357	41241	1.88%	0.317%
19	17.062	2541	2546	2555	rBV2	16905	31122	1.42%	0.239%


Sum of corrected areas: 13008925

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081320\
Data File : BF121273.D
Acq On : 13 Aug 2020 16:30
Operator : JU/CG
Sample : PB130942BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130942BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

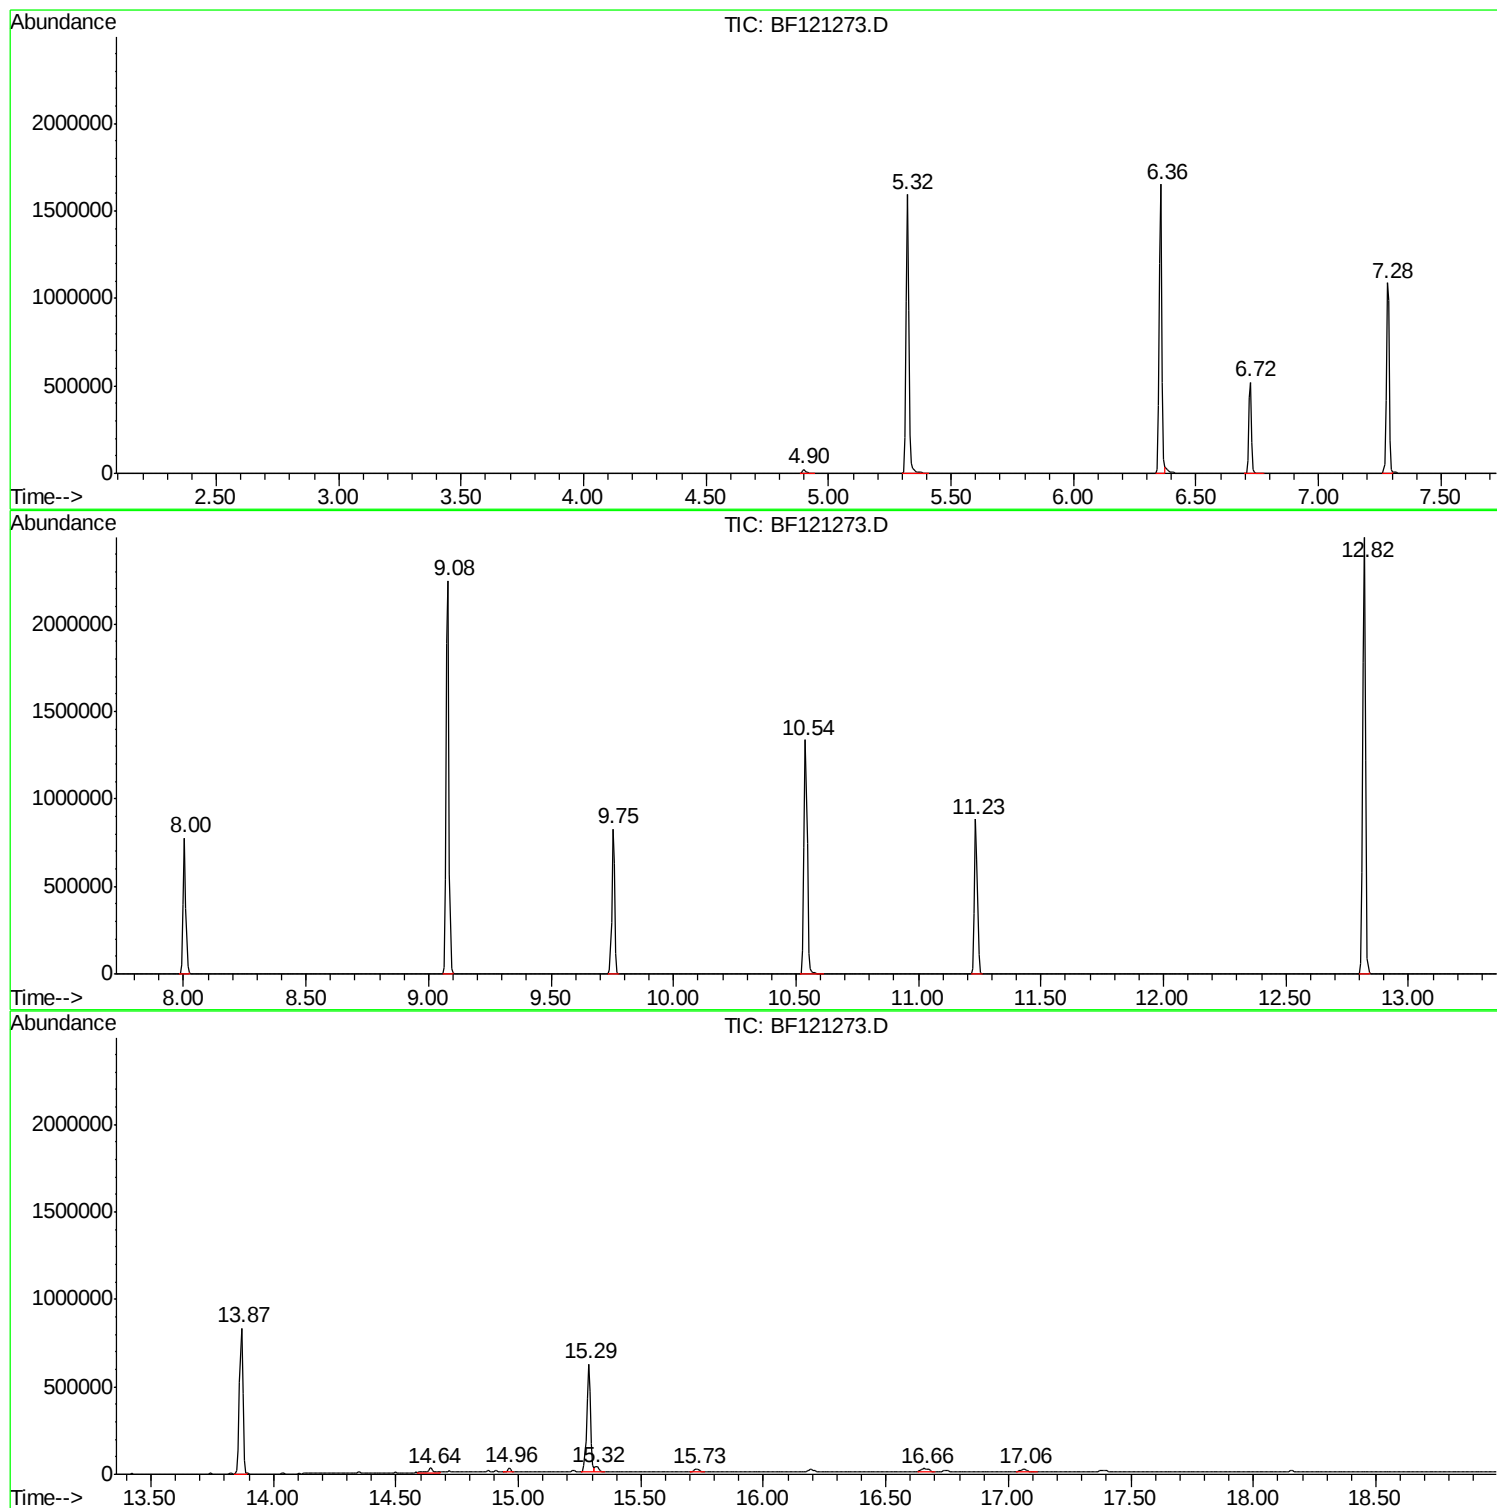

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081320\
Data File : BF121273.D
Acq On : 13 Aug 2020 16:30
Operator : JU/CG
Sample : PB130942BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130942BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF081320\
Data File : BF121273.D
Acq On : 13 Aug 2020 16:30
Operator : JU/CG
Sample : PB130942BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130942BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc