


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081320\
 Data File : BF121264.D
 Acq On : 13 Aug 2020 10:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 13 15:23:26 2020

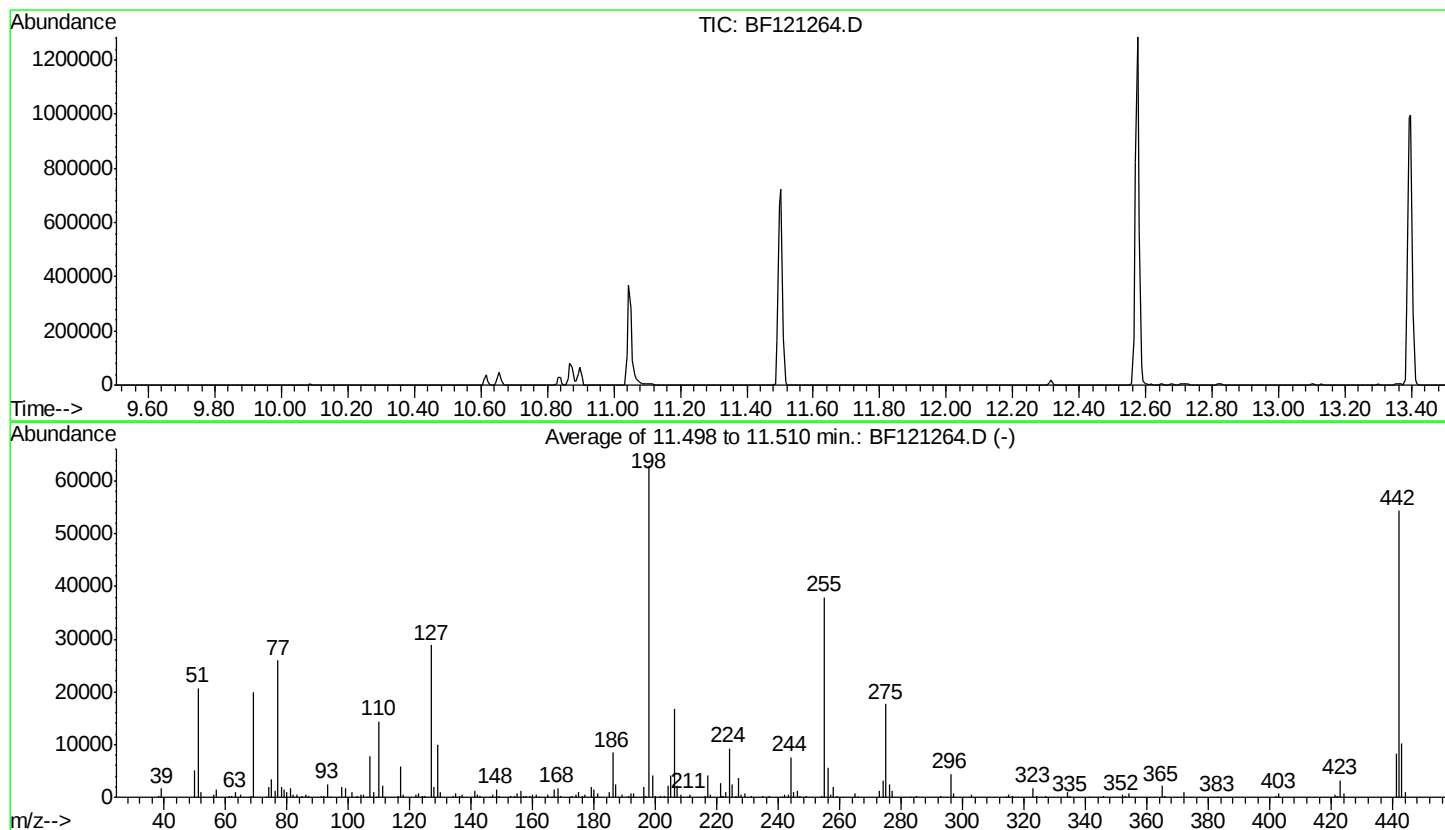

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	20713	PASS
68	69	0.00	2	1.5	299	PASS
69	198	0.00	100	31.5	19816	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.8	28832	PASS
197	198	0.00	2	0.2	121	PASS
198	198	100	100	100.0	62914	PASS
199	198	5	9	6.4	4051	PASS
275	198	10	60	28.1	17663	PASS
365	198	1	100	3.4	2138	PASS
441	198	0.01	100	13.1	8270	PASS
442	198	50	100	86.5	54392	PASS
443	442	15	24	18.7	10173	PASS