
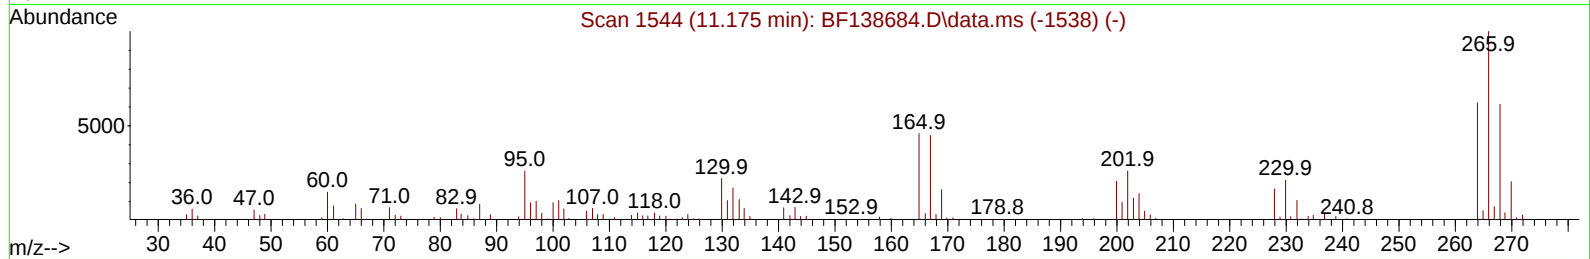
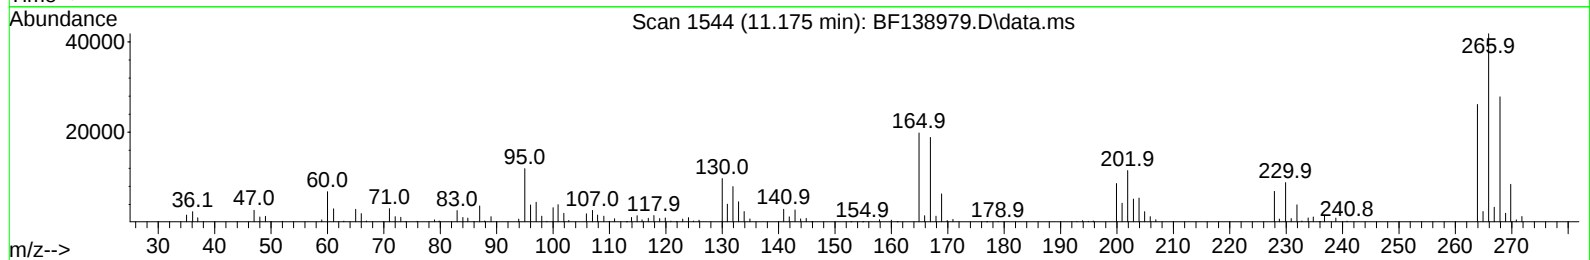


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138979.D
Acq On : 13 Aug 2024 17:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 19:02:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

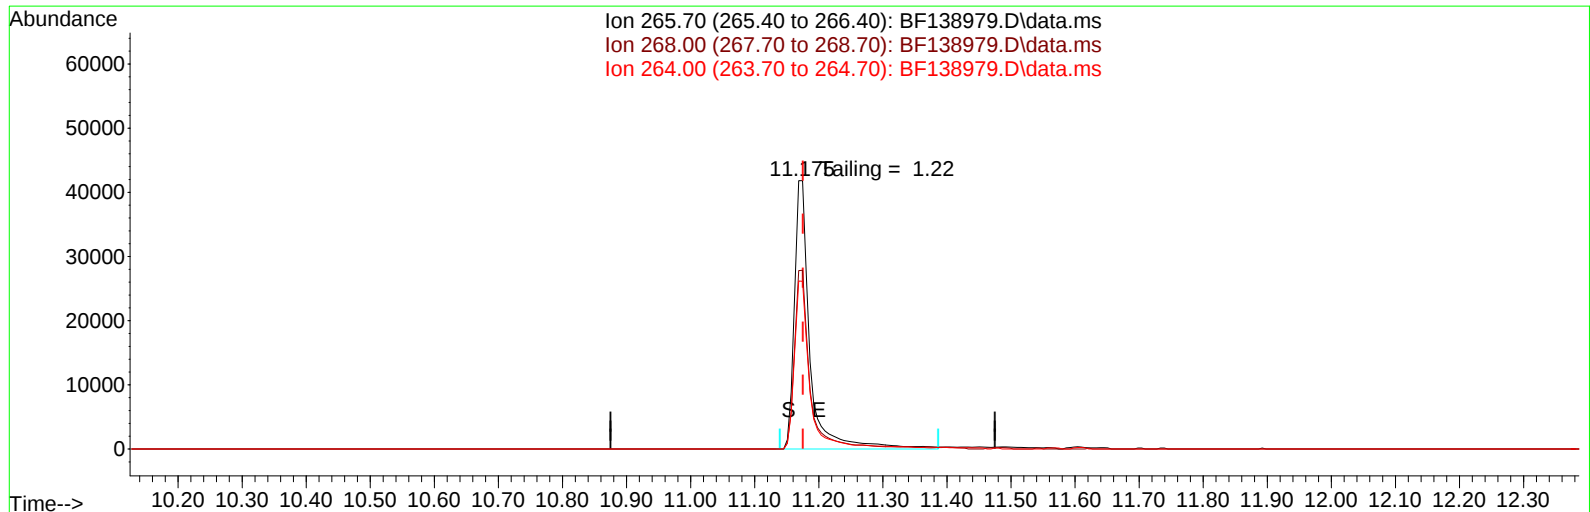

TIC: BF138979.D\data.ms

(70) Pentachlorophenol (C)




11.175min (-0.000) 254412.61 ng

response 71788

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	66.62
264.00	62.20	62.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138979.D
Acq On : 13 Aug 2024 17:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 19:02:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

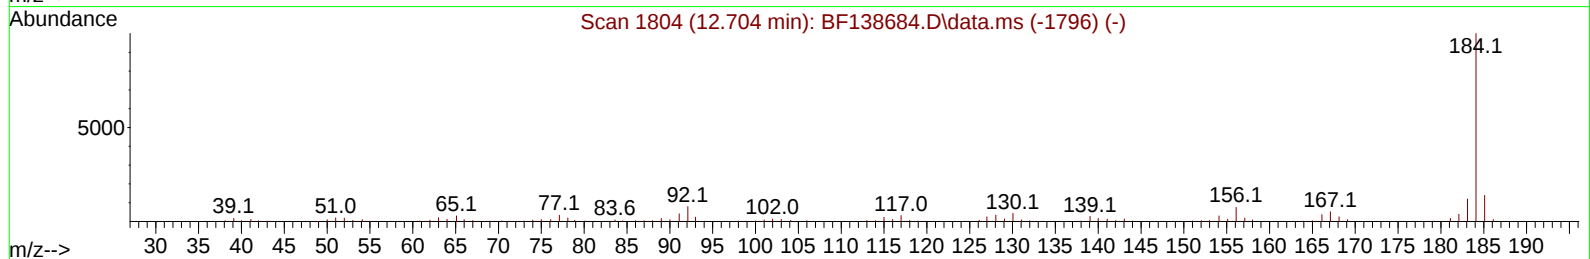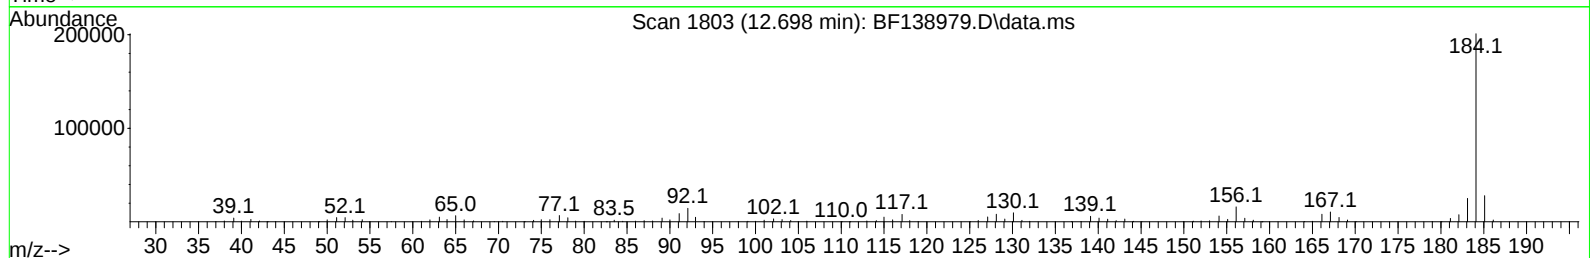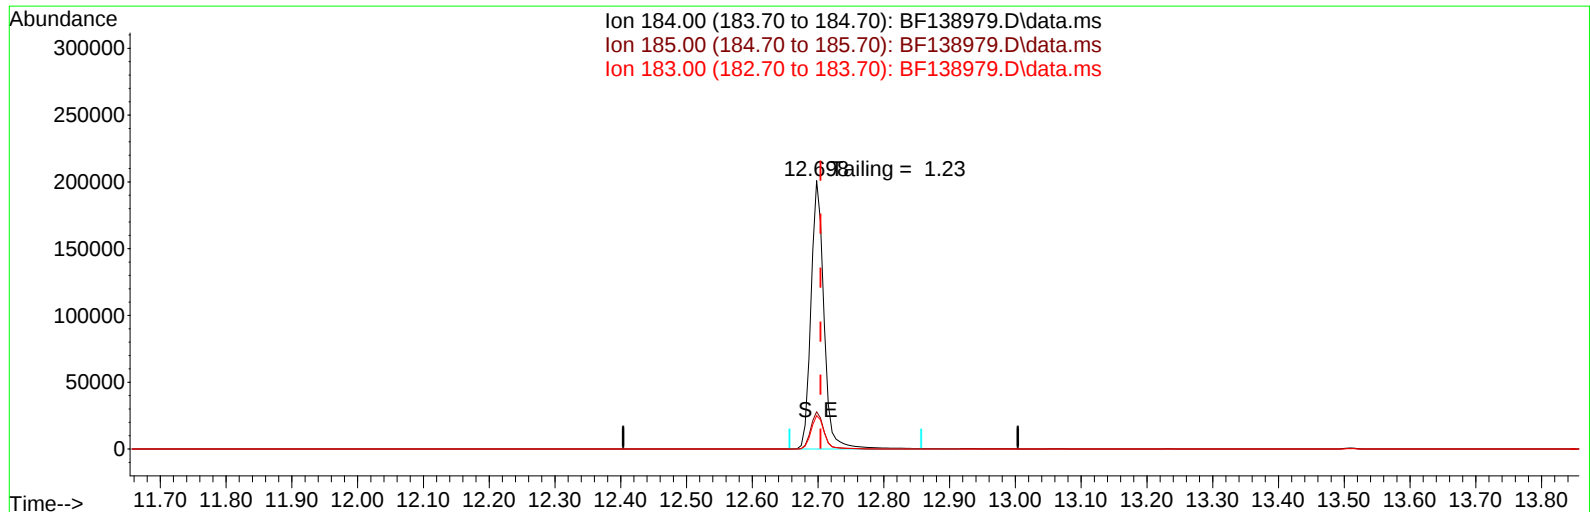

TIC: BF138979.D\data.ms

(77) Benzidine**12.698min (-0.006) 99672.07 ng****response 276542**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.93
183.00	12.00	12.48
0.00	0.00	0.00