

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
 Data File : BF138972.D
 Acq On : 13 Aug 2024 13:47
 Operator : RC/JU
 Sample : P3520-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-CF-12-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	5	15	rVB	310685	401284	55.46%	7.451%
2	5.057	500	504	522	rVB	22711	34831	4.81%	0.647%
3	5.469	569	574	599	rBV	389951	561633	77.62%	10.428%
4	6.481	741	746	768	rBV	441194	609841	84.28%	11.323%
5	6.834	802	806	814	rBB	195036	250187	34.58%	4.645%
6	7.404	898	903	916	rBV	304246	400387	55.33%	7.434%
7	8.116	1019	1024	1042	rBV	259878	328536	45.40%	6.100%
8	8.439	1075	1079	1093	rBV	11195	18858	2.61%	0.350%
9	9.186	1201	1206	1217	rBV	567298	723579	100.00%	13.435%
10	9.869	1317	1322	1332	rBV	289733	360899	49.88%	6.701%
11	9.963	1332	1338	1349	rVB	89348	137525	19.01%	2.553%
12	10.663	1452	1457	1471	rBV	252496	348999	48.23%	6.480%
13	11.357	1570	1575	1592	rVB	259258	326552	45.13%	6.063%
14	12.933	1838	1843	1849	rBV	400616	506789	70.04%	9.410%
15	13.845	1991	1998	2013	rBV5	6113	23278	3.22%	0.432%
16	13.998	2019	2024	2032	rBV	141730	185061	25.58%	3.436%
17	15.462	2267	2273	2286	rVB	100017	167648	23.17%	3.113%




Sum of corrected areas: 5385887

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138972.D
Acq On : 13 Aug 2024 13:47
Operator : RC/JU
Sample : P3520-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-12-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

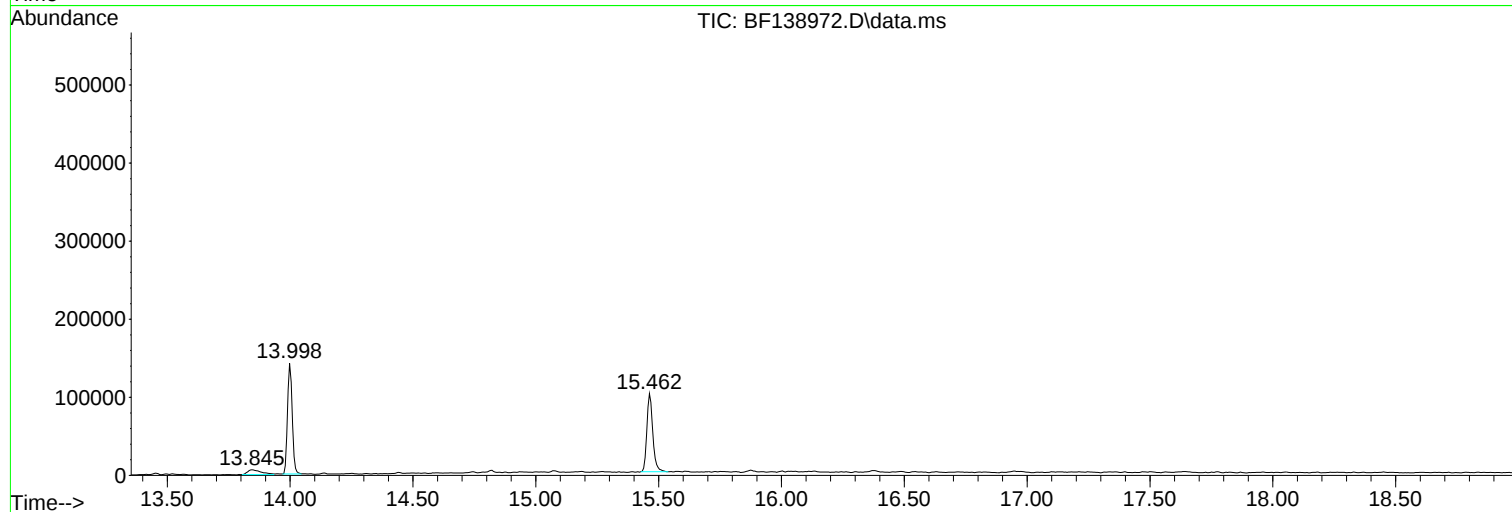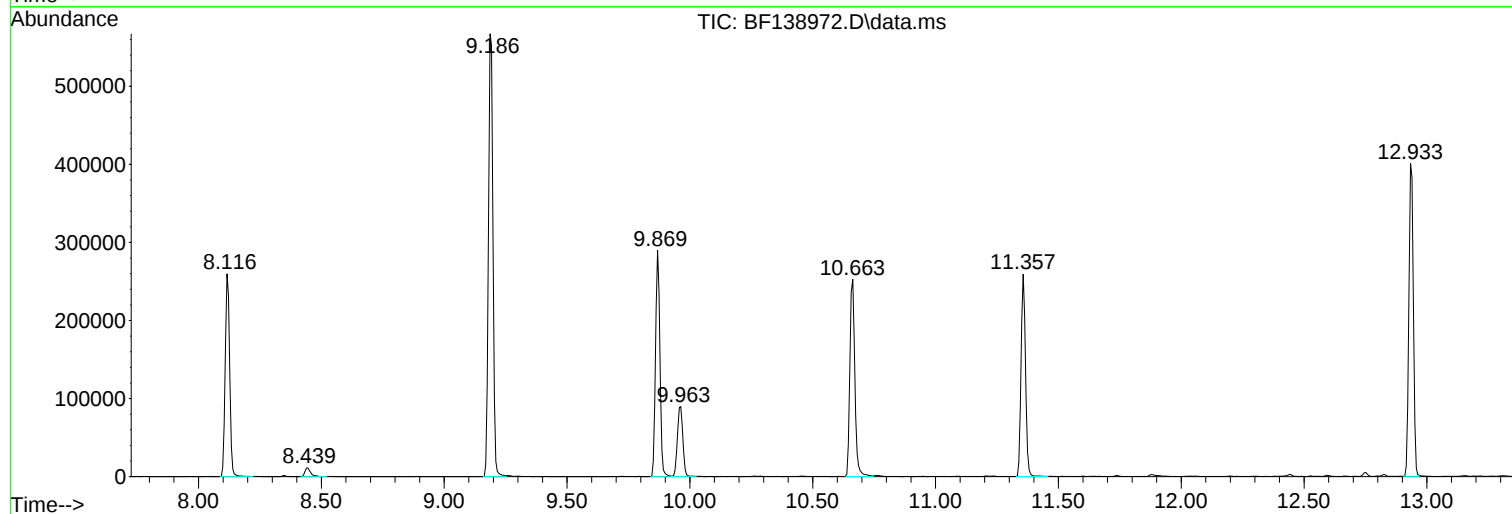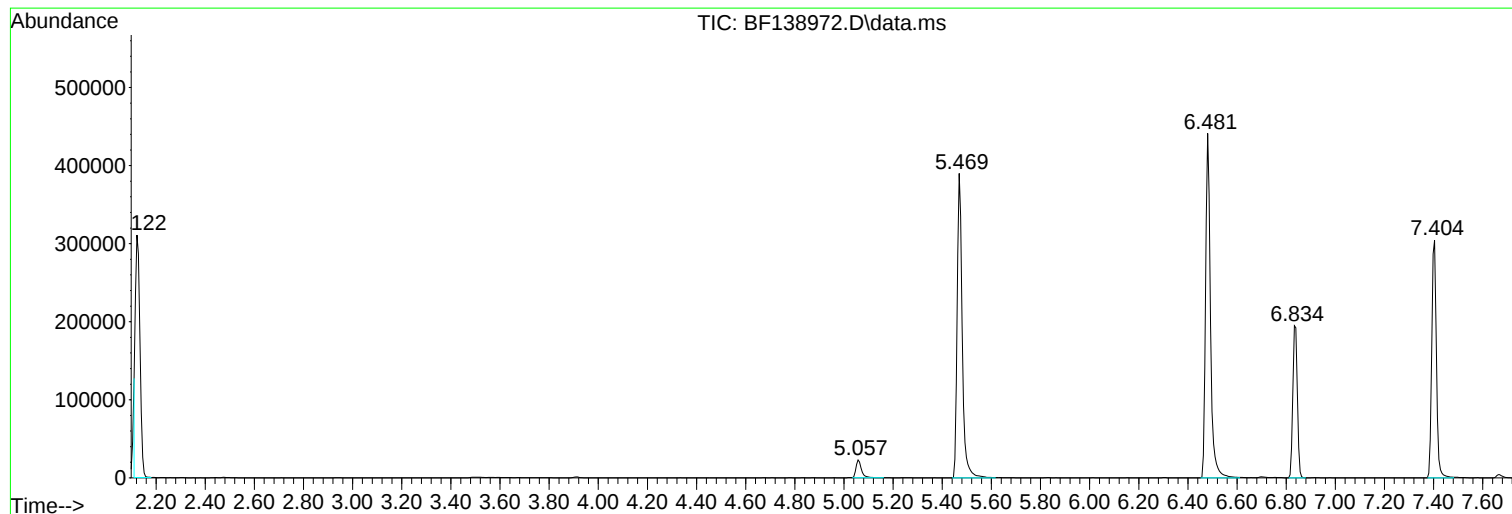

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138972.D
Acq On : 13 Aug 2024 13:47
Operator : RC/JU
Sample : P3520-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-12-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138972.D
Acq On : 13 Aug 2024 13:47
Operator : RC/JU
Sample : P3520-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-12-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------