

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
 Data File : BF138975.D
 Acq On : 13 Aug 2024 15:19
 Operator : RC/JU
 Sample : P3519-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-CF-01-080624

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.158	3	11	24	rVB	649605	1002697	60.01%	8.850%
2	3.416	221	225	265	rBV	18604	59399	3.55%	0.524%
3	5.075	501	507	523	rVB	121622	217749	13.03%	1.922%
4	5.475	570	575	598	rBV	1073141	1489421	89.13%	13.146%
5	6.487	741	747	774	rBV	1136131	1567281	93.79%	13.833%
6	6.681	774	780	792	rBV	12747	25154	1.51%	0.222%
7	6.840	802	807	812	rBV	212384	270846	16.21%	2.390%
8	7.404	897	903	917	rBV	759822	1029545	61.61%	9.087%
9	8.116	1019	1024	1040	rBV	285186	358576	21.46%	3.165%
10	8.440	1074	1079	1090	rBV	23947	38315	2.29%	0.338%
11	9.192	1201	1207	1212	rBV	1331555	1671016	100.00%	14.748%
12	9.869	1317	1322	1332	rBV	315120	386674	23.14%	3.413%
13	9.963	1332	1338	1350	rVV	333144	496445	29.71%	4.382%
14	10.663	1452	1457	1467	rBV	690070	902291	54.00%	7.964%
15	11.357	1570	1575	1584	rBV	274140	341334	20.43%	3.013%
16	12.939	1838	1844	1849	rBV	854519	1071499	64.12%	9.457%
17	13.839	1990	1997	2008	rBV4	12379	39411	2.36%	0.348%
18	13.998	2019	2024	2034	rVB	142753	187185	11.20%	1.652%
19	15.463	2267	2273	2287	rVB	104167	175376	10.50%	1.548%




Sum of corrected areas: 11330214

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138975.D
Acq On : 13 Aug 2024 15:19
Operator : RC/JU
Sample : P3519-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-01-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

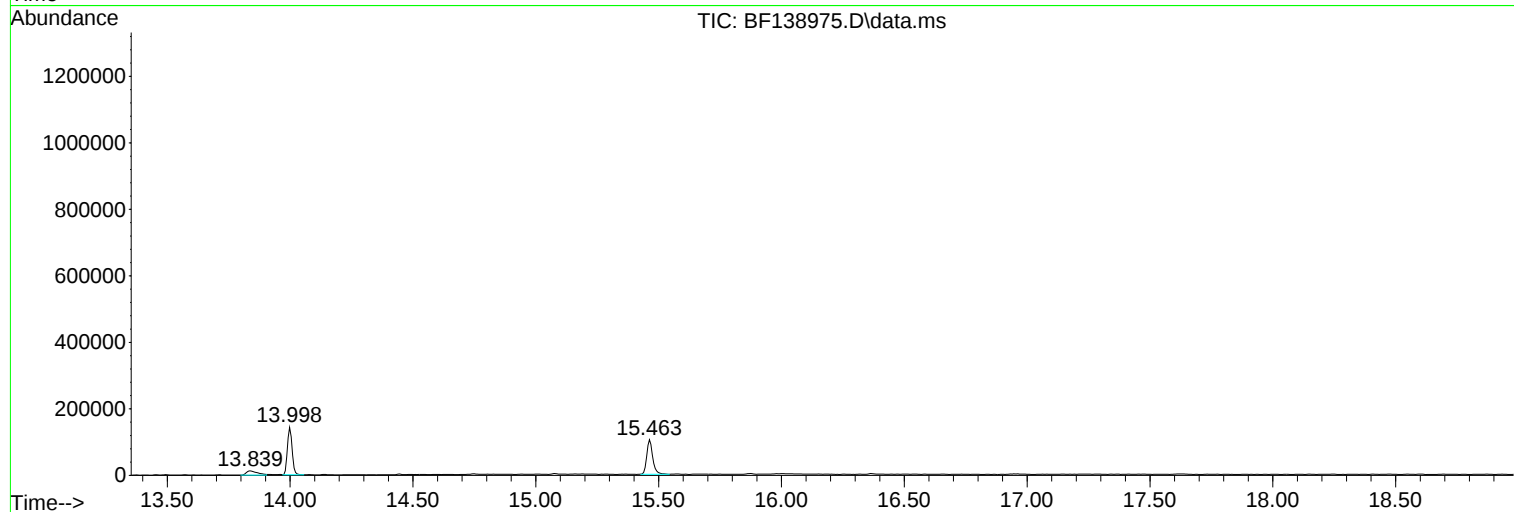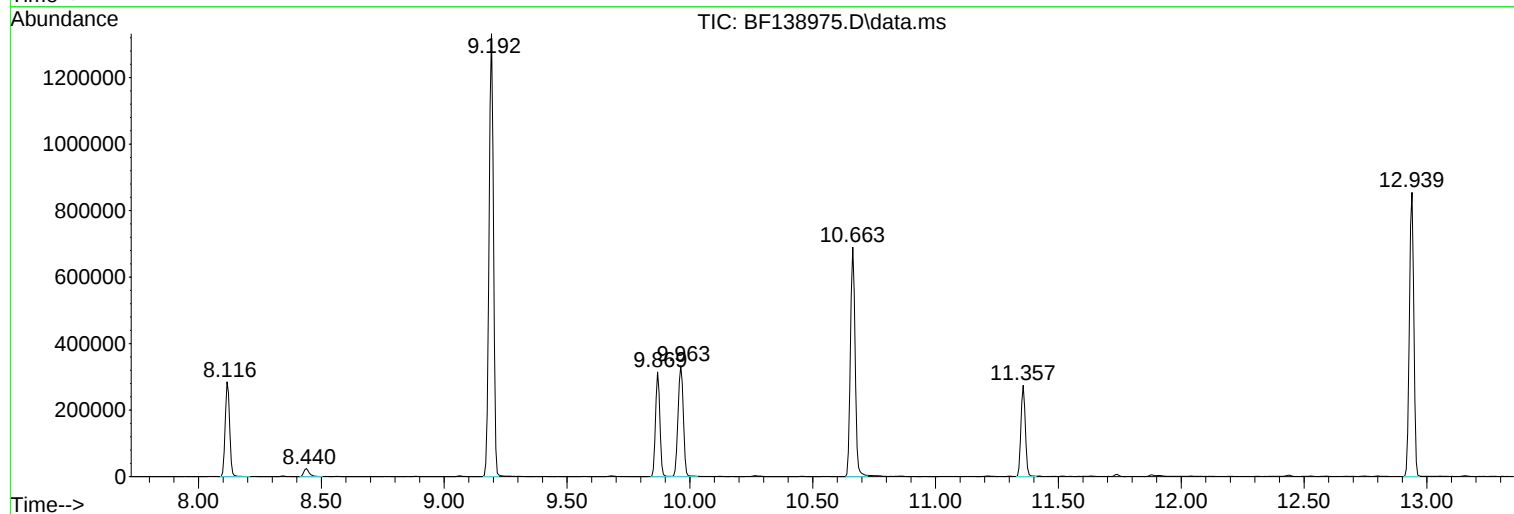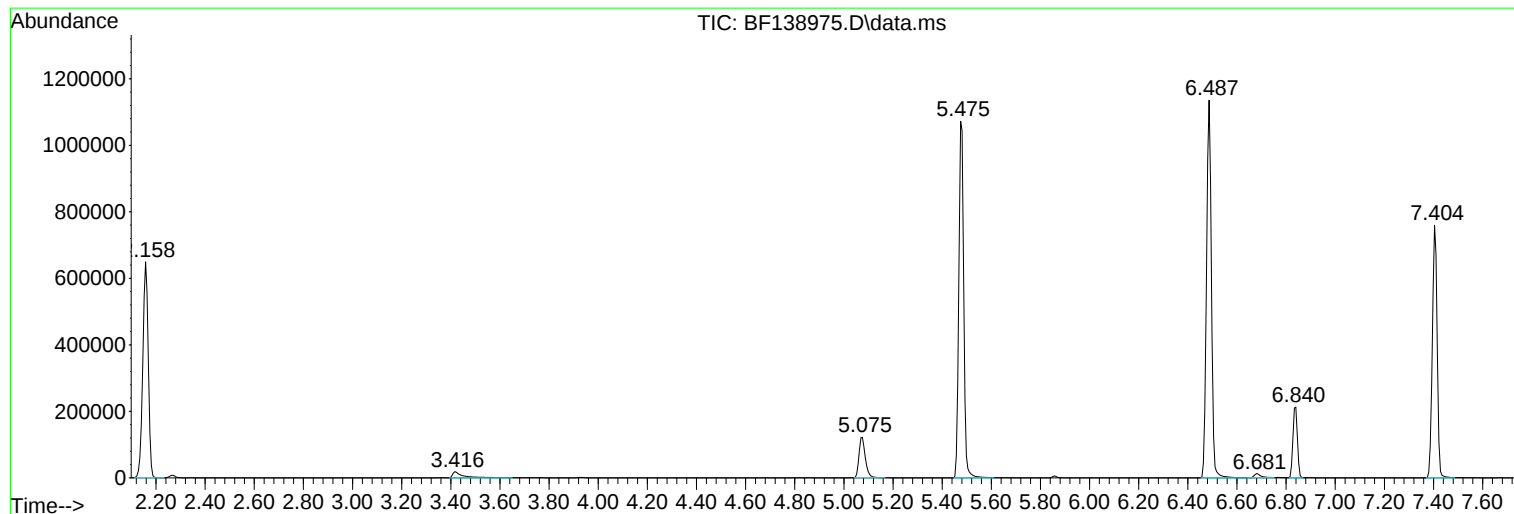

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138975.D
Acq On : 13 Aug 2024 15:19
Operator : RC/JU
Sample : P3519-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-01-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138975.D
Acq On : 13 Aug 2024 15:19
Operator : RC/JU
Sample : P3519-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-CF-01-080624

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------