


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138979.D
Acq On : 13 Aug 2024 17:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

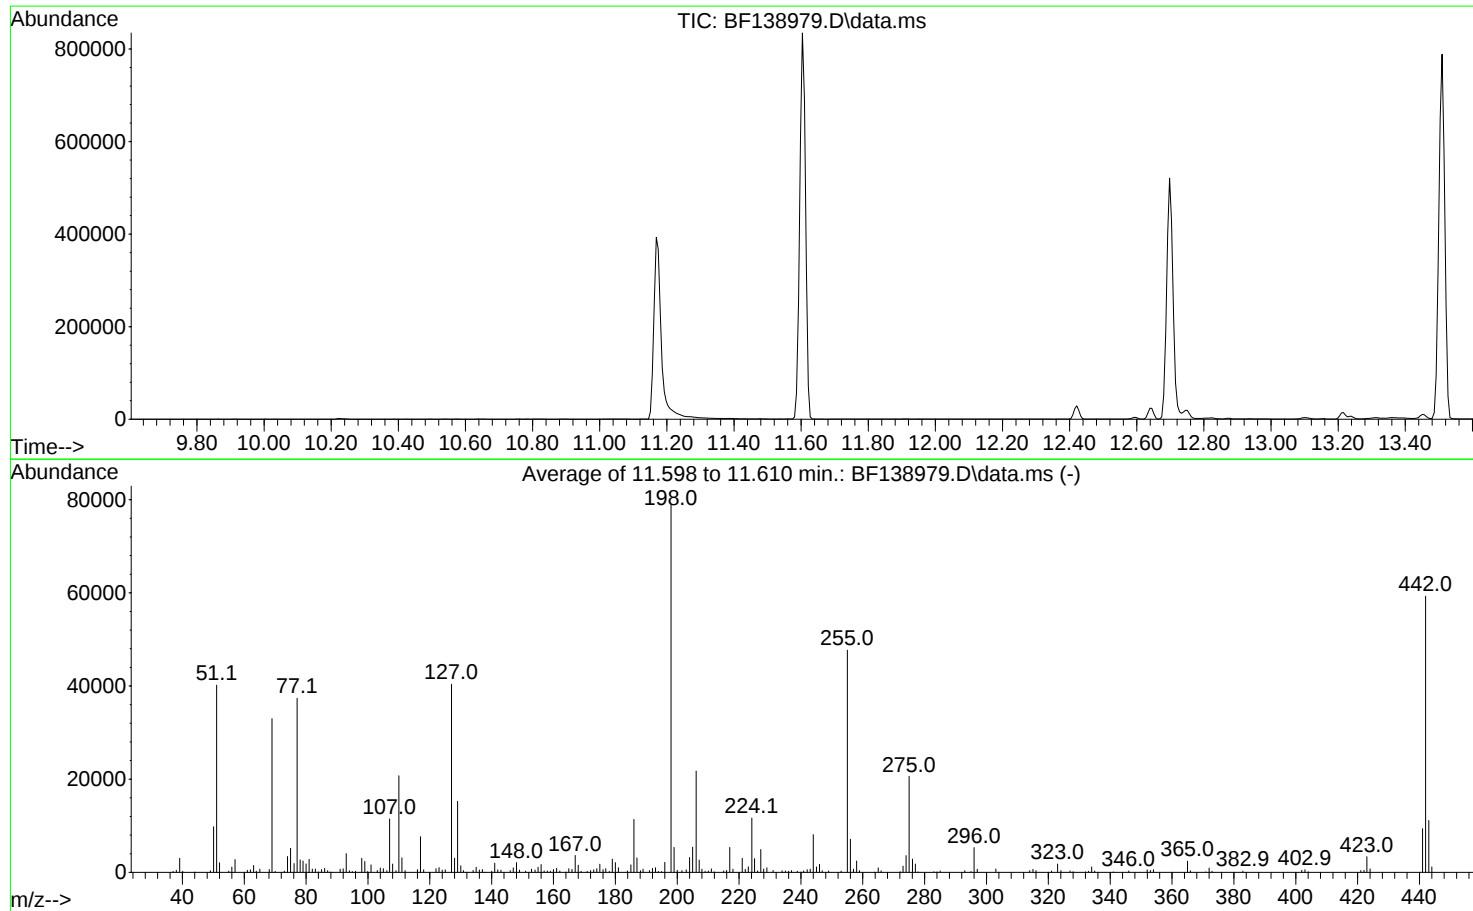

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.9	40197	PASS
68	69	0.00	2	1.9	635	PASS
69	198	0.00	100	41.8	32997	PASS
70	69	0.00	2	0.6	196	PASS
127	198	10	80	51.1	40389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78963	PASS
199	198	5	9	6.8	5349	PASS
275	198	10	60	26.1	20601	PASS
365	198	1	100	3.1	2423	PASS
441	198	0.01	100	11.9	9390	PASS
442	442	50	100	100.0	59285	PASS
443	442	15	24	18.8	11130	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/13/2024	BNA_F	<u>BF138979.D</u>
Compound Name	Response	Retention Time
DDT	184956	13.51
DDD	6822	13.216
DDE	651	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7473	192429	3.88

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\
Data File : BF138979.D
Acq On : 13 Aug 2024 17:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 19:02:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

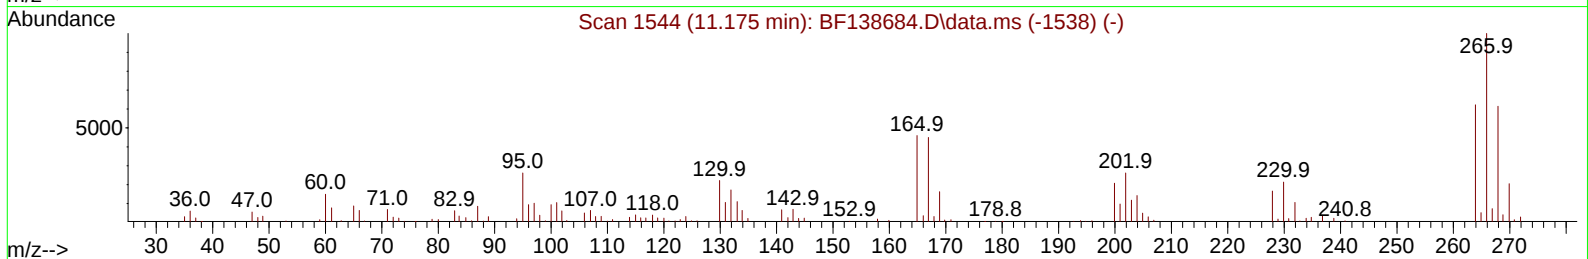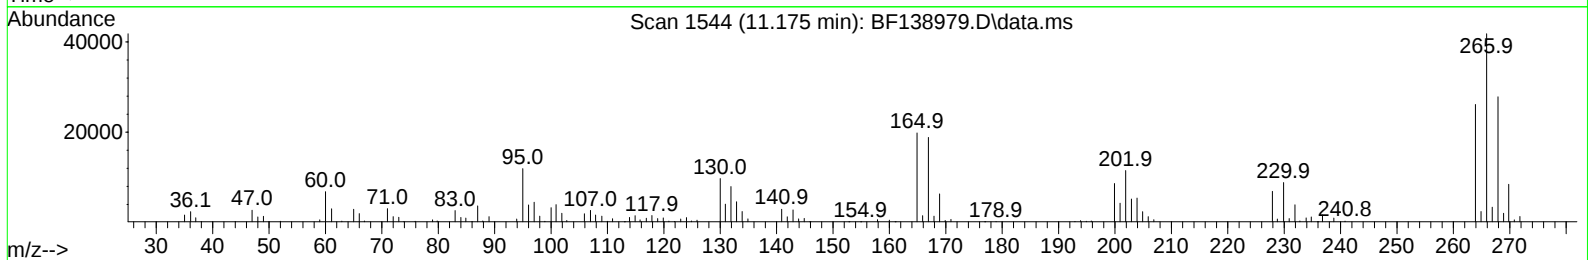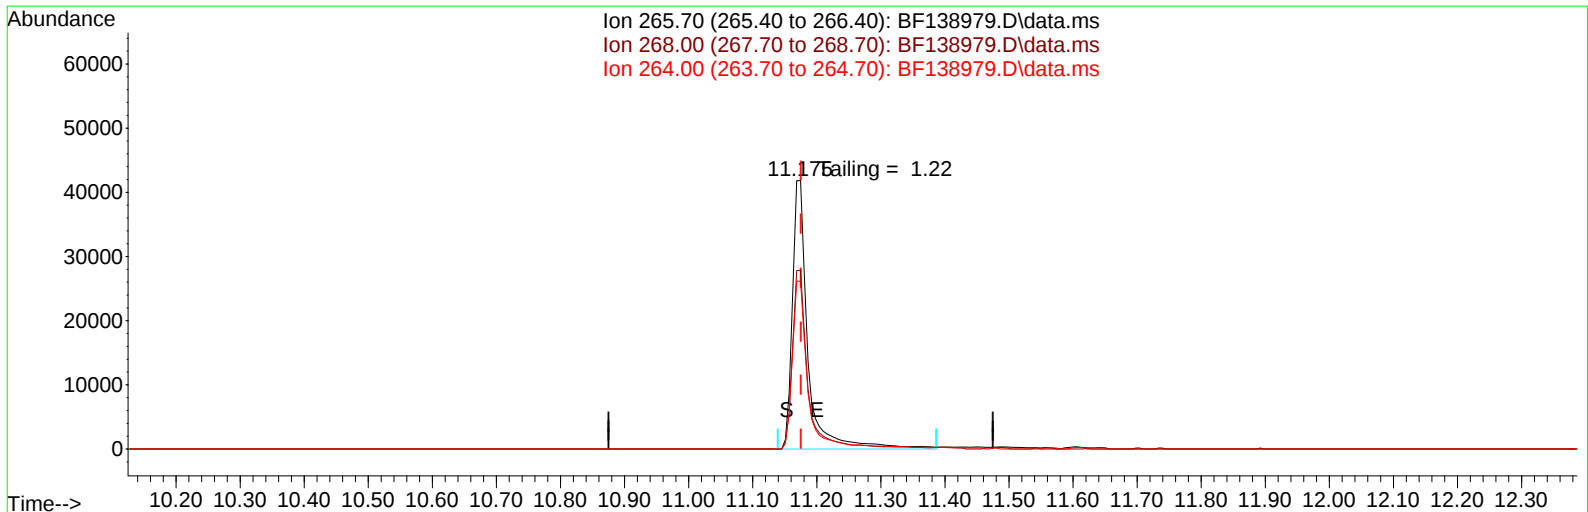

TIC: BF138979.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 254412.61 ng




response 71788

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	66.62
264.00	62.20	62.49
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081324\  
Data File : BF138979.D  
Acq On    : 13 Aug 2024 17:59  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 13 19:02:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

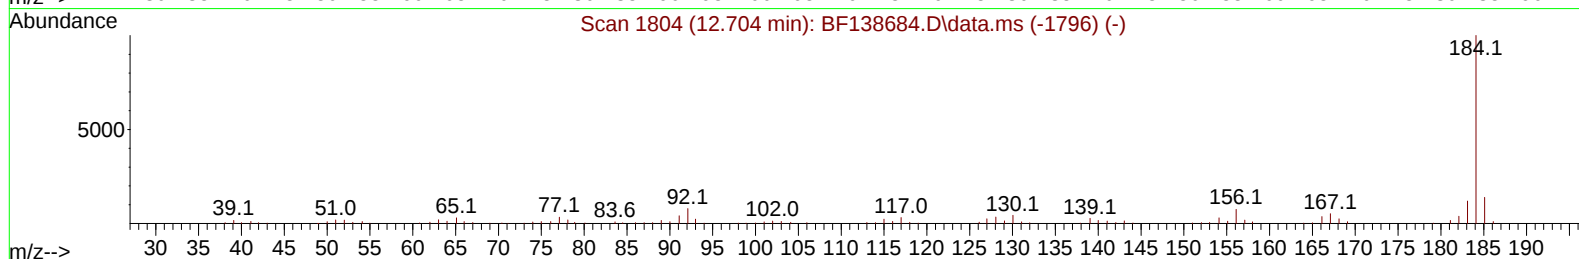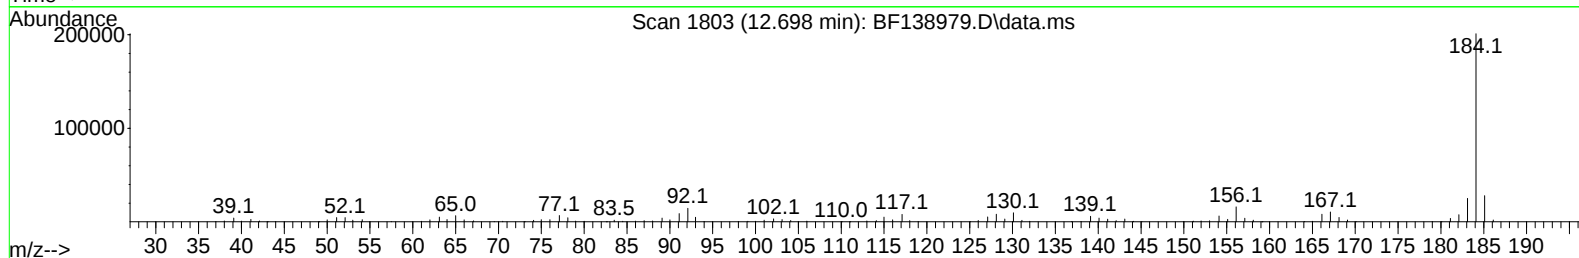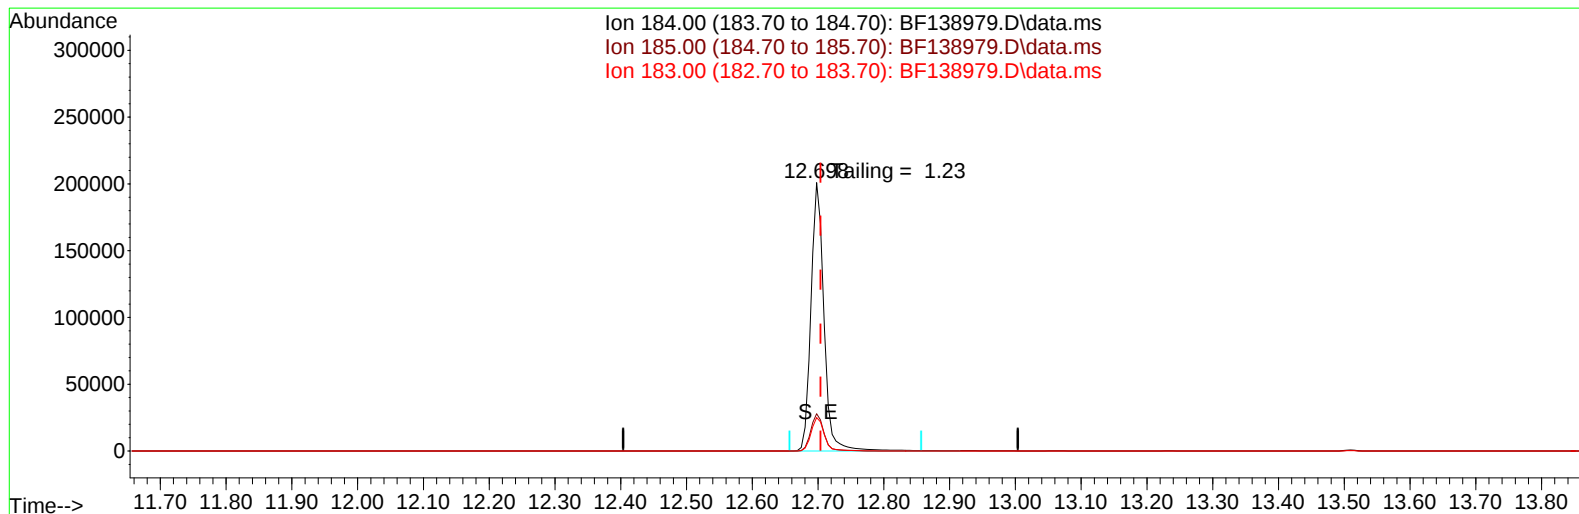

TIC: BF138979.D\data.ms

(77) Benzidine

12.698min (-0.006) 99672.07 ng

response **276542**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.93
183.00	12.00	12.48
0.00	0.00	0.00