
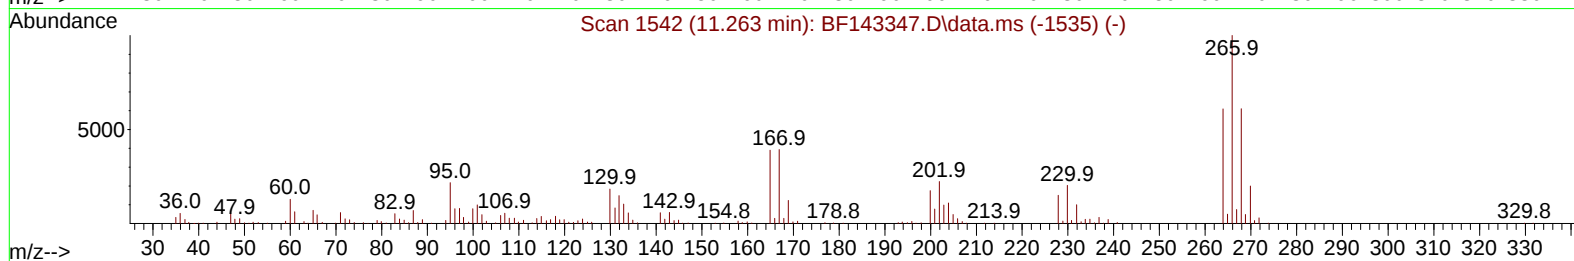
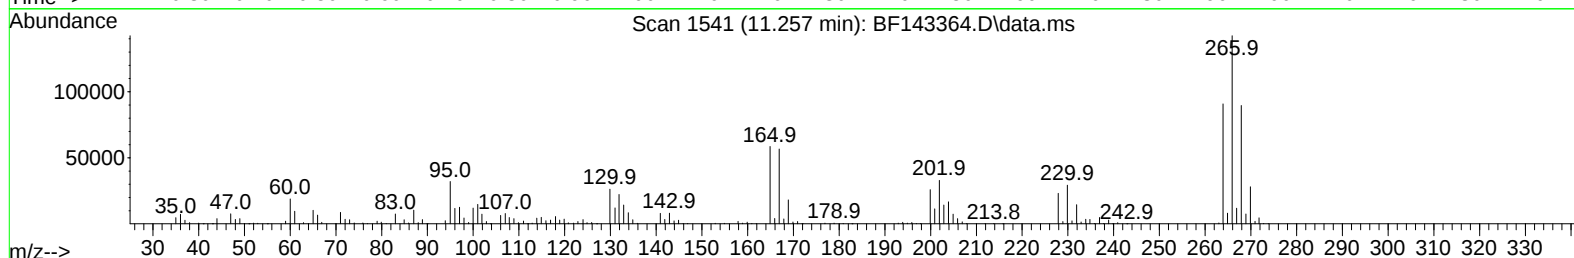


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081325\
Data File : BF143364.D
Acq On : 13 Aug 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 11:48:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

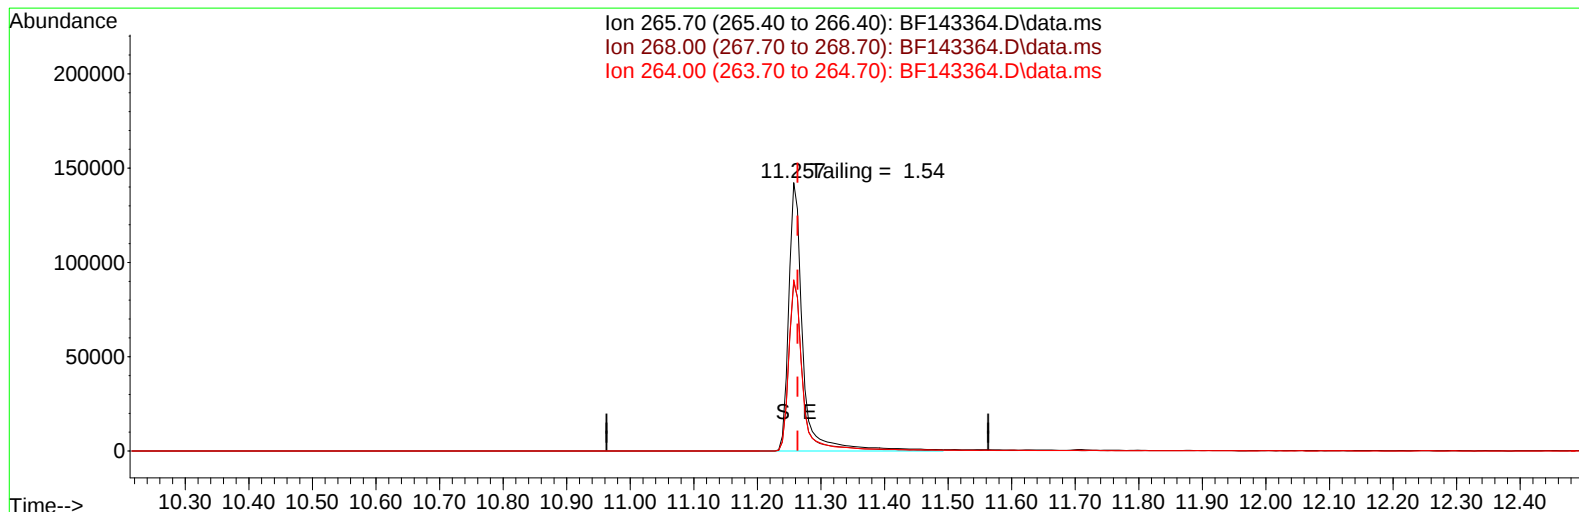

TIC: BF143364.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.006) 27752.57 ng

response 221678

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	62.96
264.00	61.00	63.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081325\
Data File : BF143364.D
Acq On : 13 Aug 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 13 11:48:18 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

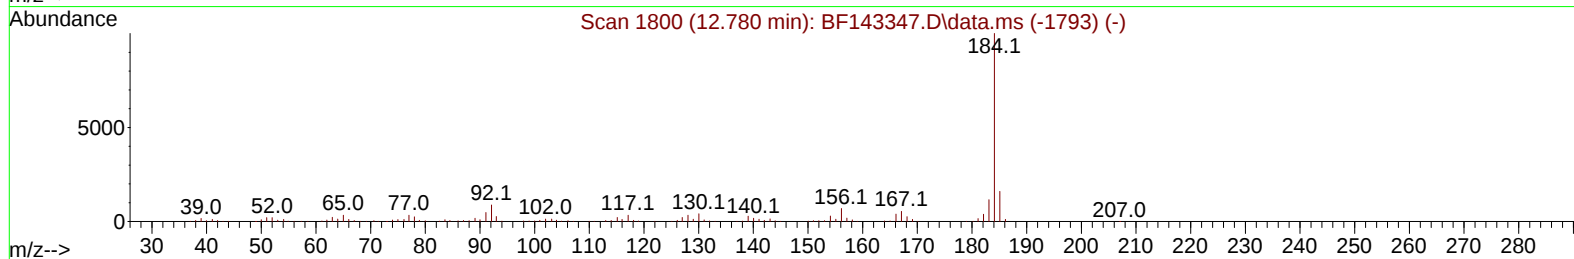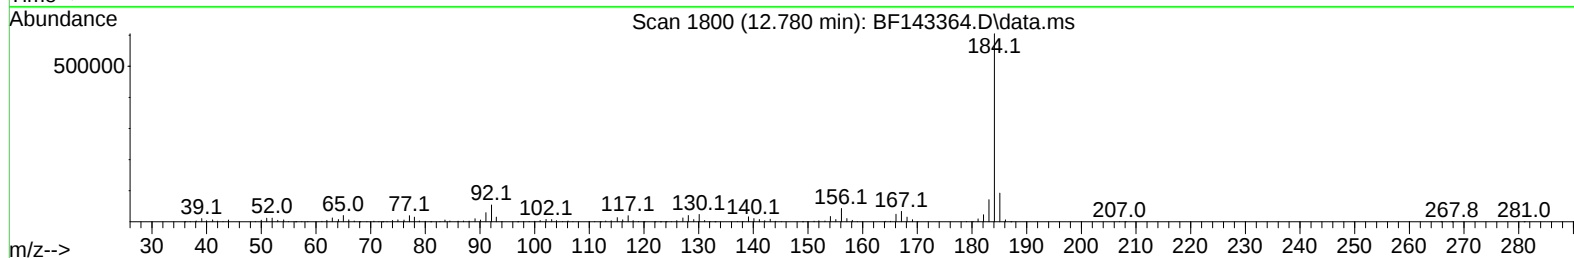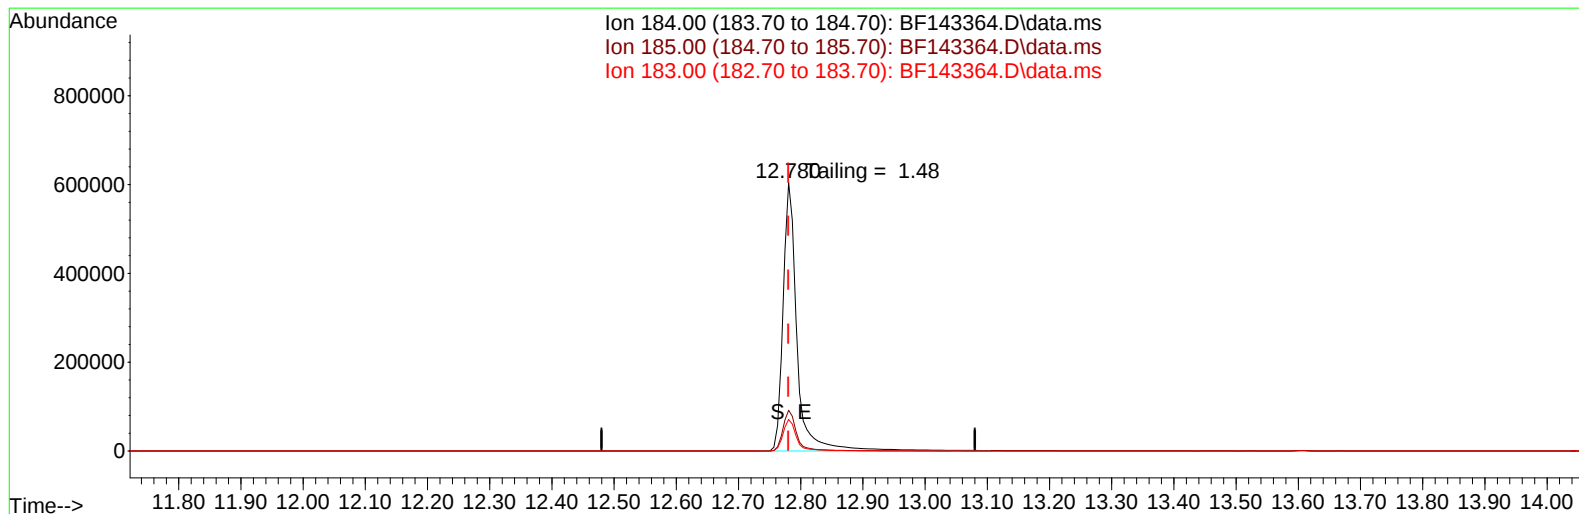

TIC: BF143364.D\data.ms

(77) Benzidine

12.780min (+ 0.000) 0.00 ng

response 949077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	15.22
183.00	11.60	11.79
0.00	0.00	0.00