
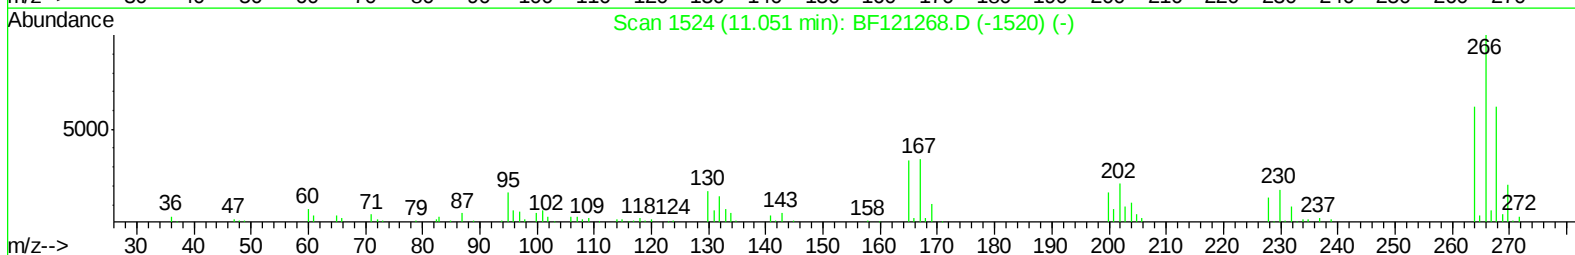
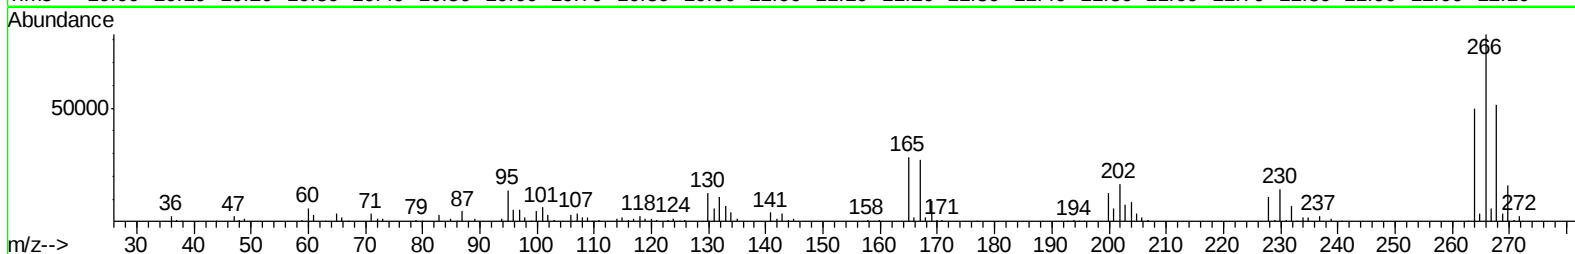


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081420\
 Data File : BF121287.D
 Acq On : 14 Aug 2020 15:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 05:11:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 13 15:23:26 2020
 Response via : Initial Calibration

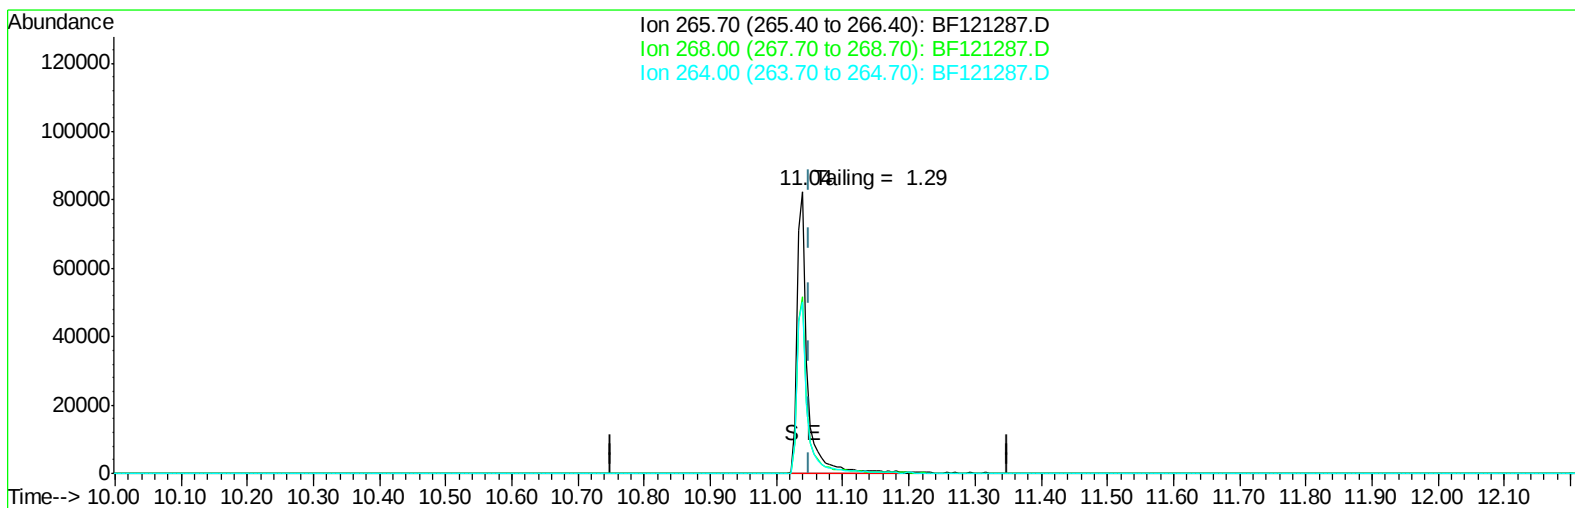

TIC: BF121287.D

(70) Pentachlorophenol (C)




11.039min (-0.011) 106580.03ng

response 91149

Ion	Exp%	Act%
265.70	100	100
268.00	63.70	62.60
264.00	63.30	60.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081420\
 Data File : BF121287.D
 Acq On : 14 Aug 2020 15:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 05:11:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF081320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 13 15:23:26 2020
 Response via : Initial Calibration

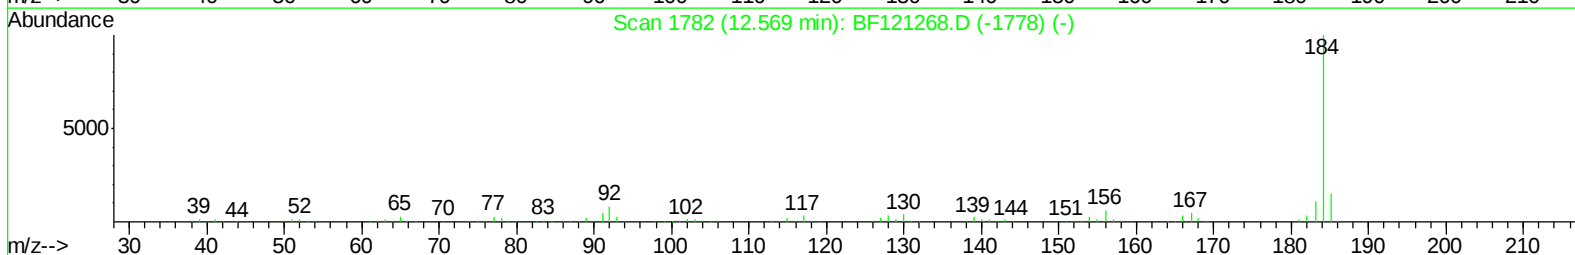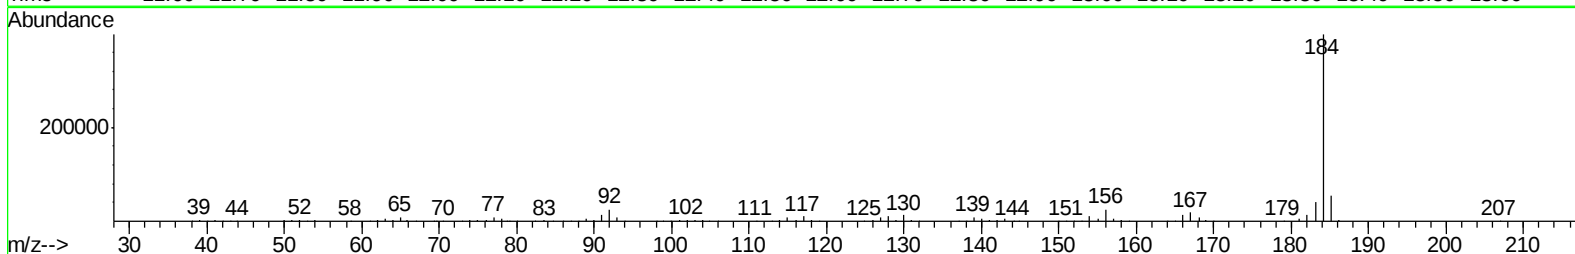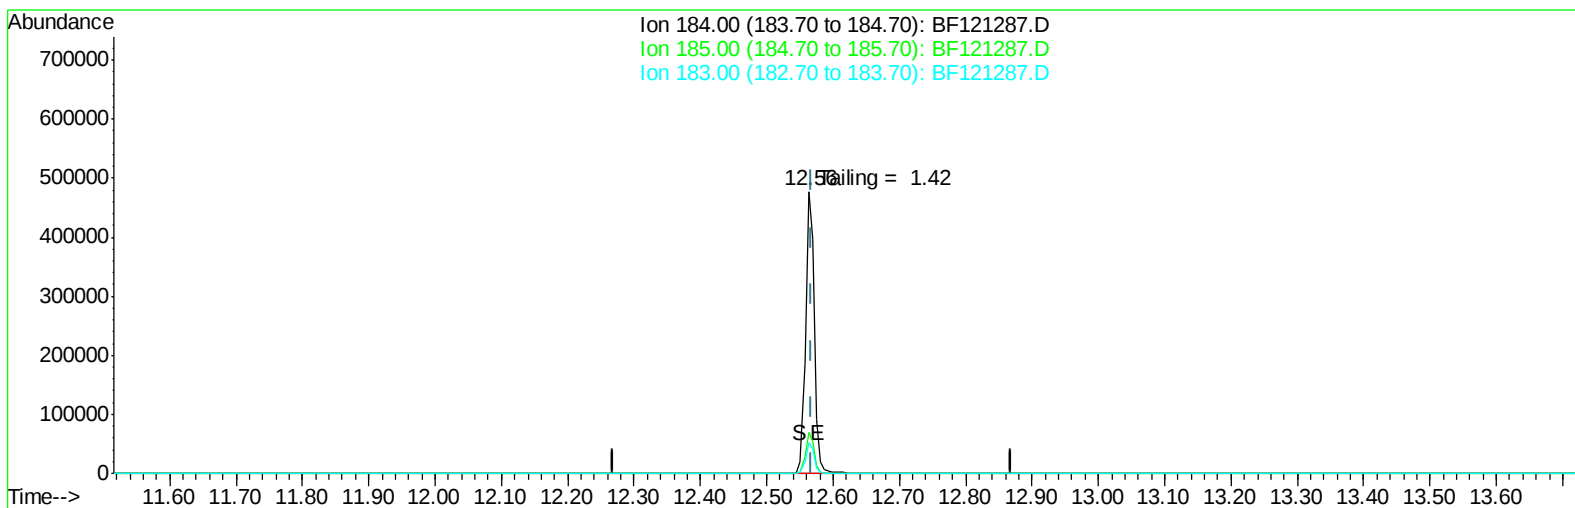

TIC: BF121287.D

(77) Benzidine

12.563min (-0.006) 27814.16ng

response 430677

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.54
183.00	10.40	11.05
0.00	0.00	0.00