


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081420\
 Data File : BF121287.D
 Acq On : 14 Aug 2020 15:34
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081320.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 13 15:23:26 2020

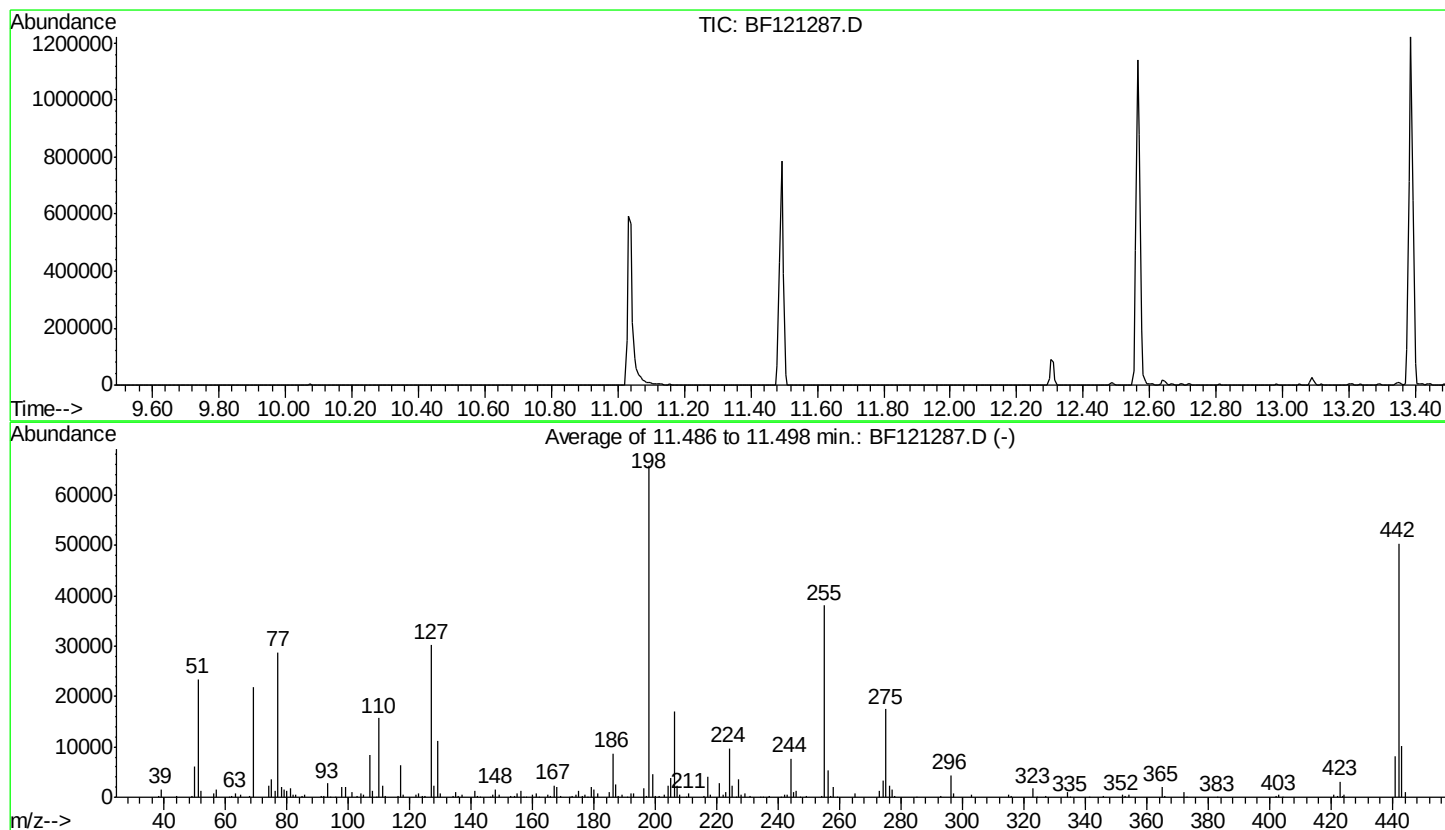

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	23406	PASS
68	69	0.00	2	1.4	305	PASS
69	198	0.00	100	33.1	21765	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	30357	PASS
197	198	0.00	2	0.5	340	PASS
198	198	100	100	100.0	65826	PASS
199	198	5	9	7.0	4600	PASS
275	198	10	60	26.5	17447	PASS
365	198	1	100	3.1	2056	PASS
441	198	0.01	100	12.4	8137	PASS
442	198	50	100	76.6	50434	PASS
443	442	15	24	20.0	10081	PASS