
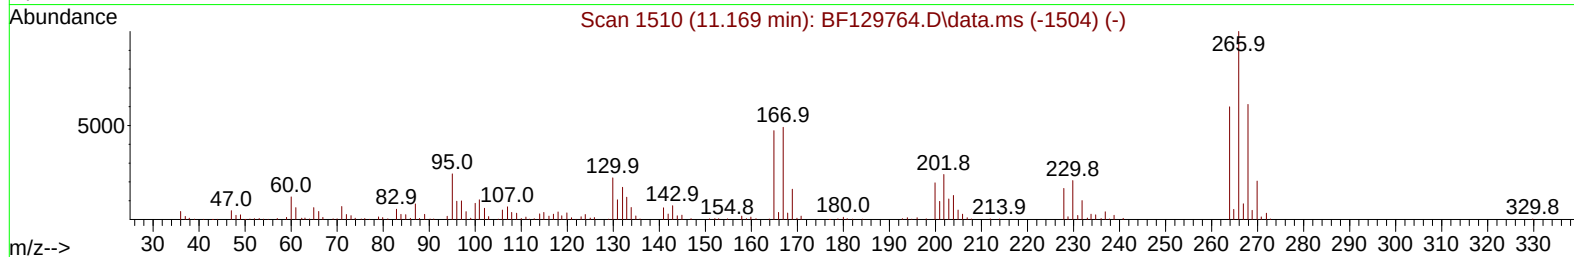
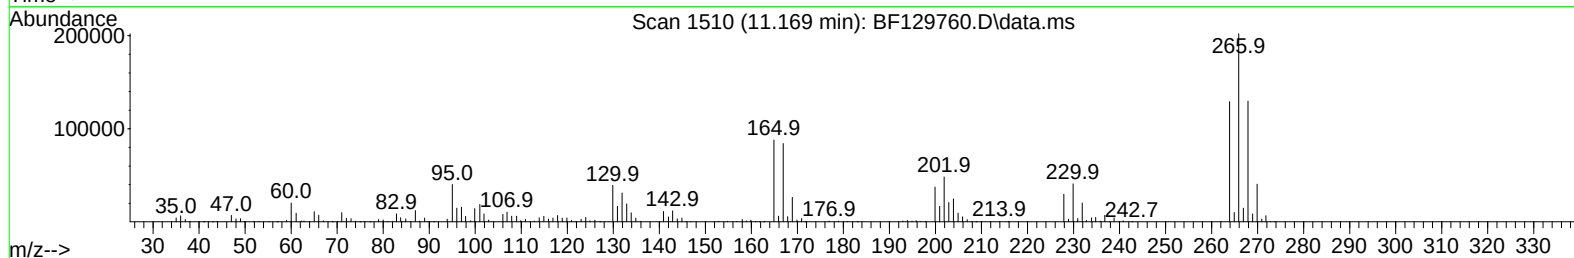


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
 Data File : BF129760.D
 Acq On : 14 Aug 2022 13:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 05:53:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 15 02:28:31 2022
 Response via : Initial Calibration

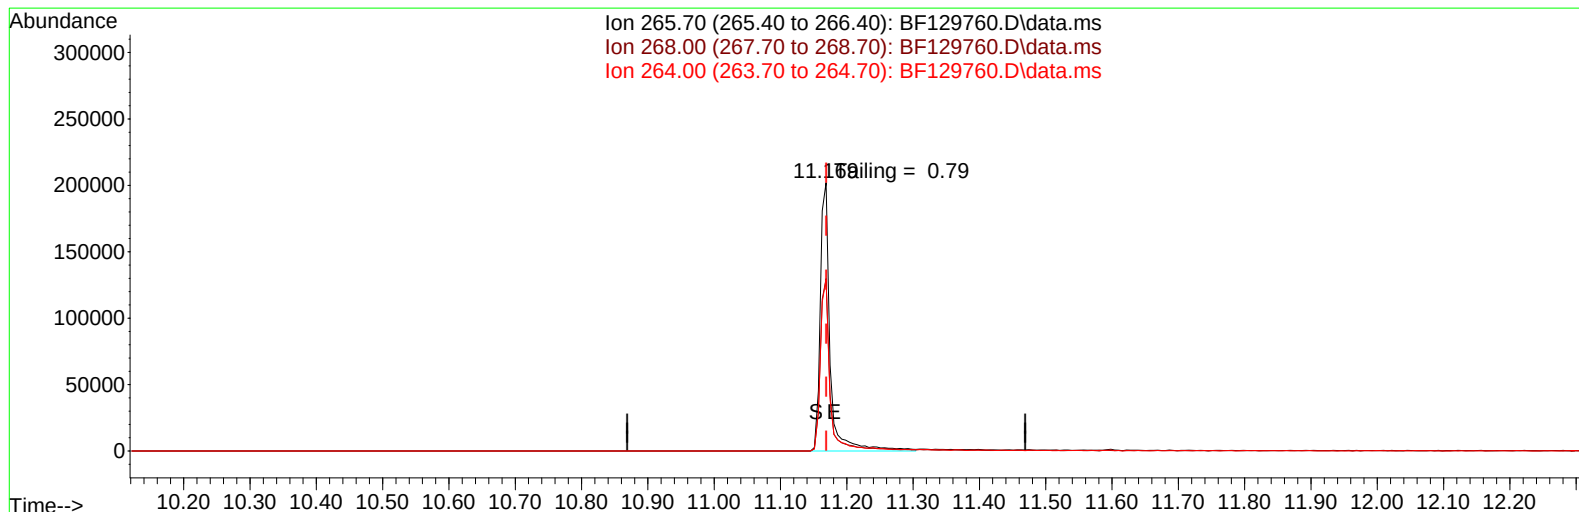

TIC: BF129760.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.000) 106918.19 ng

response 210859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.17
264.00	59.90	63.98
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\  
Data File : BF129760.D  
Acq On    : 14 Aug 2022  13:35  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Aug 15 05:53:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

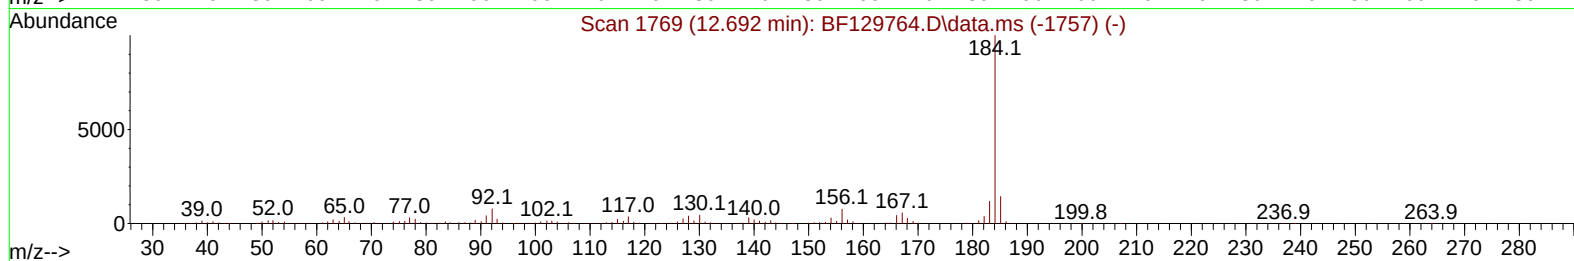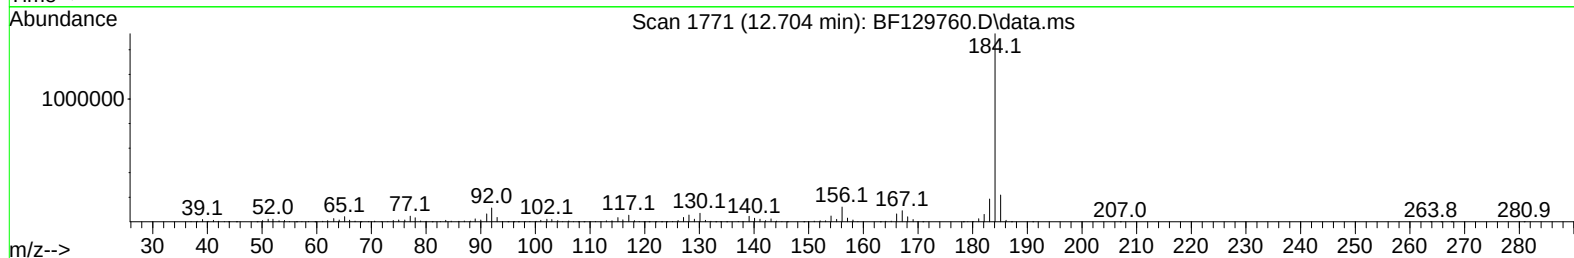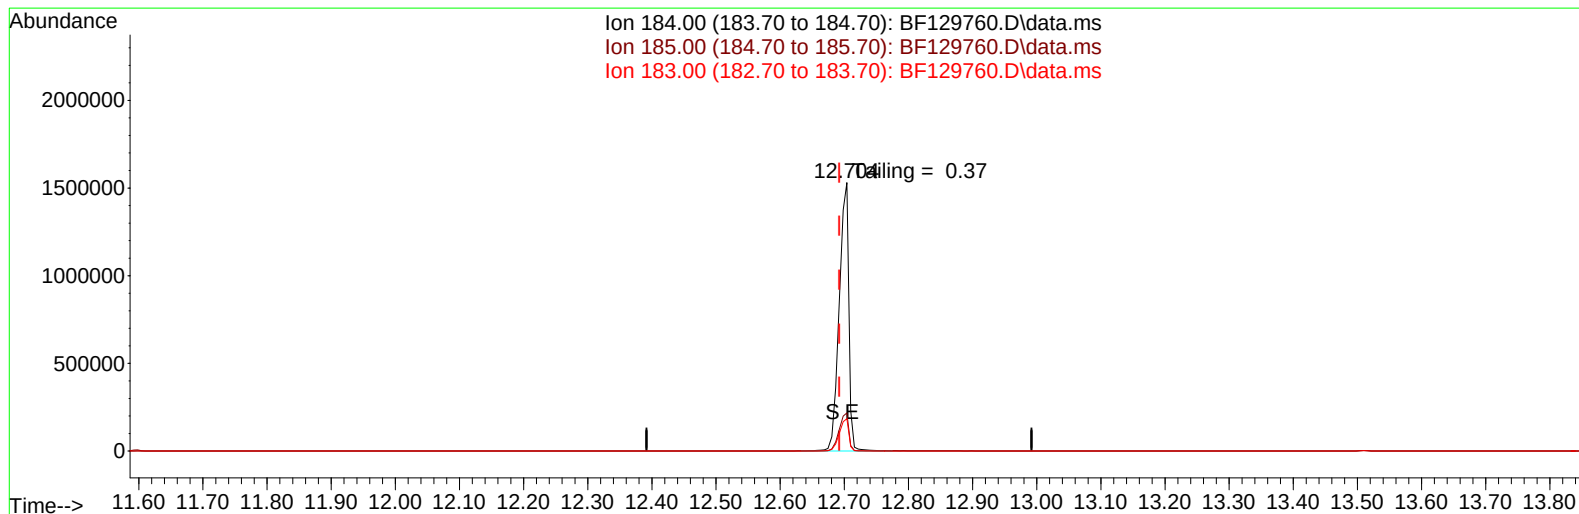

TIC: BF129760.D\data.ms

(77) Benzidine

12.704min (+ 0.012) 75643.92 ng

response **1610819**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.19
183.00	11.80	12.07
0.00	0.00	0.00