

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
 Data File : BF129775.D
 Acq On : 14 Aug 2022 21:58
 Operator : CG\JU
 Sample : PB146963BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146963BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129775.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	537	541	556	rBV	4142015	4157431	68.47%	12.303%
2	6.481	708	713	732	rBV	3944108	4202608	69.22%	12.436%
3	6.822	767	771	775	rBV	1077064	951485	15.67%	2.816%
4	7.392	862	868	871	rBV	2441111	2770296	45.63%	8.198%
5	8.104	984	989	992	rBV	1366415	1301940	21.44%	3.853%
6	9.181	1166	1172	1175	rBV	5288027	5380385	88.61%	15.921%
7	9.857	1282	1287	1291	rBV	1623139	1522957	25.08%	4.507%
8	10.657	1418	1423	1426	rBV	3786099	3337928	54.98%	9.878%
9	11.351	1537	1541	1544	rBV	1970696	1593845	26.25%	4.716%
10	12.939	1806	1811	1814	rBV	6139297	6071659	100.00%	17.967%
11	13.998	1987	1991	1995	rBV	1639808	1397965	23.02%	4.137%
12	15.468	2233	2241	2247	rBV	875327	1104742	18.20%	3.269%




Sum of corrected areas: 33793241

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129775.D
Acq On : 14 Aug 2022 21:58
Operator : CG\JU
Sample : PB146963BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146963BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

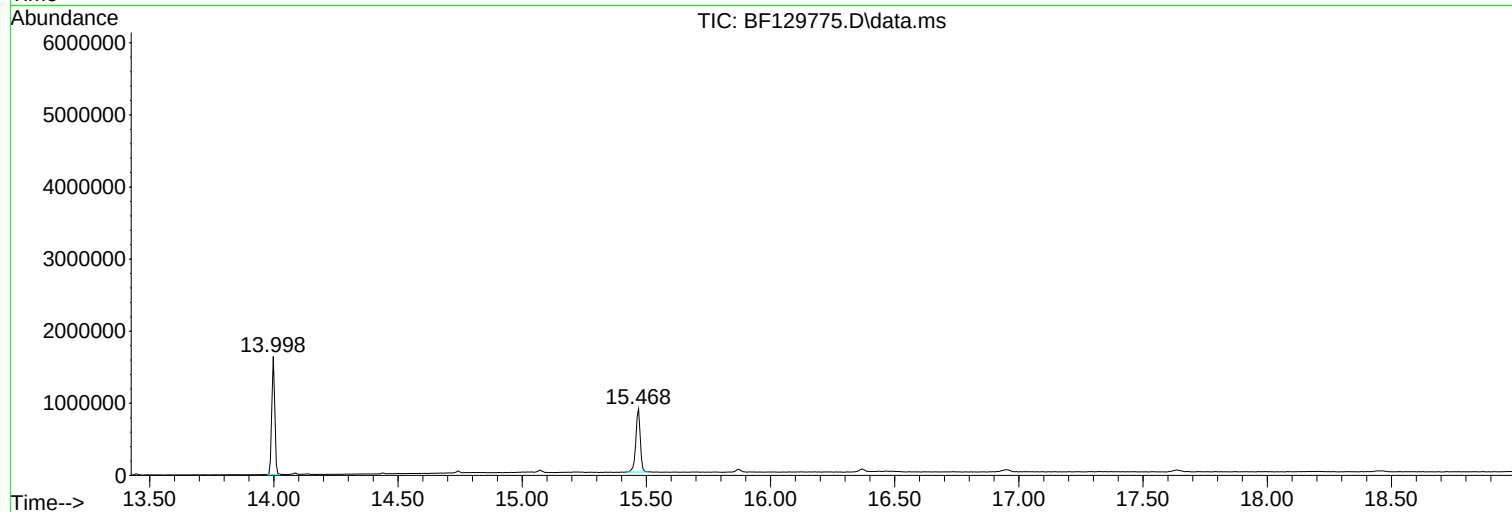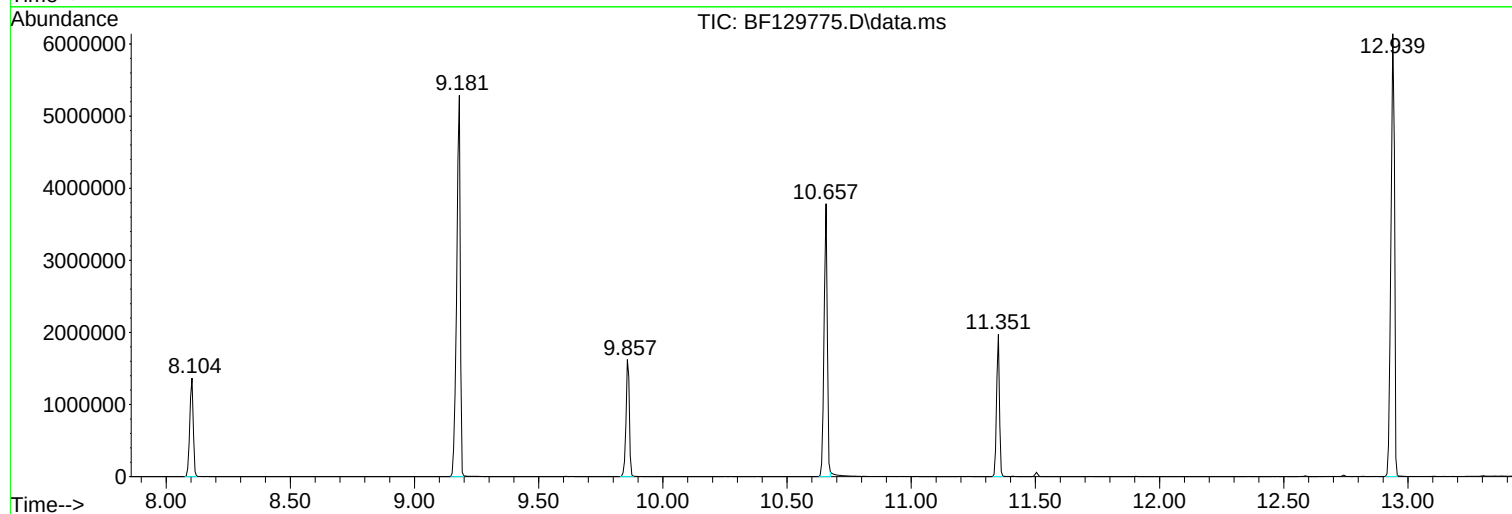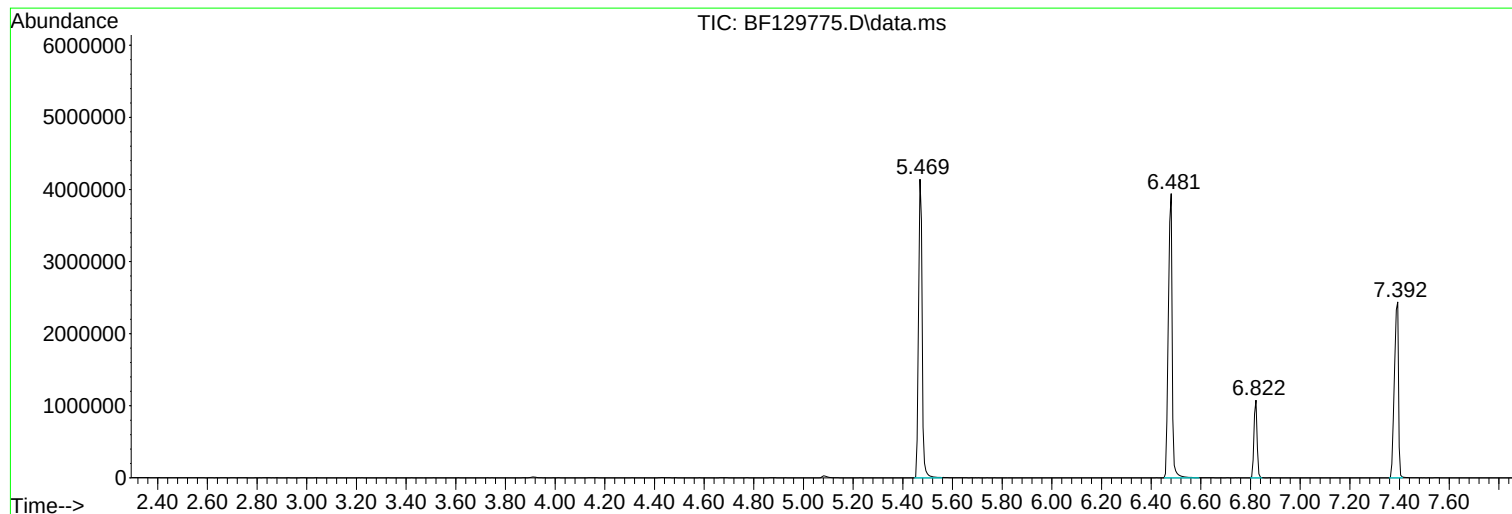

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129775.D
Acq On : 14 Aug 2022 21:58
Operator : CG\JU
Sample : PB146963BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146963BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129775.D
Acq On : 14 Aug 2022 21:58
Operator : CG\JU
Sample : PB146963BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146963BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------