

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
 Data File : BF129778.D
 Acq On : 14 Aug 2022 23:32
 Operator : CG\JU
 Sample : PB146737BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146737BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	537	541	563	rBV	4243000	4046195	68.22%	12.207%
2	6.481	708	713	736	rBV	3813386	4113774	69.36%	12.410%
3	6.822	767	771	774	rBV	1107463	927873	15.64%	2.799%
4	7.392	862	868	871	rBV	2424351	2699406	45.51%	8.144%
5	8.104	984	989	992	rBV	1330089	1266336	21.35%	3.820%
6	9.181	1166	1172	1175	rBV	5407489	5259569	88.68%	15.867%
7	9.857	1282	1287	1291	rBV	1529392	1496620	25.23%	4.515%
8	10.657	1418	1423	1426	rBV	3611263	3176281	53.56%	9.582%
9	11.351	1537	1541	1544	rBV	1866960	1556514	26.24%	4.696%
10	12.939	1806	1811	1814	rBV	6075133	5930838	100.00%	17.892%
11	13.998	1987	1991	1995	rBV	1560249	1340979	22.61%	4.045%
12	15.468	2233	2241	2249	rBV	833117	1056876	17.82%	3.188%
13	15.868	2305	2309	2314	rBV2	40455	65211	1.10%	0.197%
14	16.368	2389	2394	2400	rBV2	39612	67587	1.14%	0.204%
15	16.945	2488	2492	2501	rVB2	37255	77872	1.31%	0.235%
16	17.633	2605	2609	2620	rVB4	27097	65613	1.11%	0.198%




Sum of corrected areas: 33147544

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129778.D
Acq On : 14 Aug 2022 23:32
Operator : CG\JU
Sample : PB146737BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

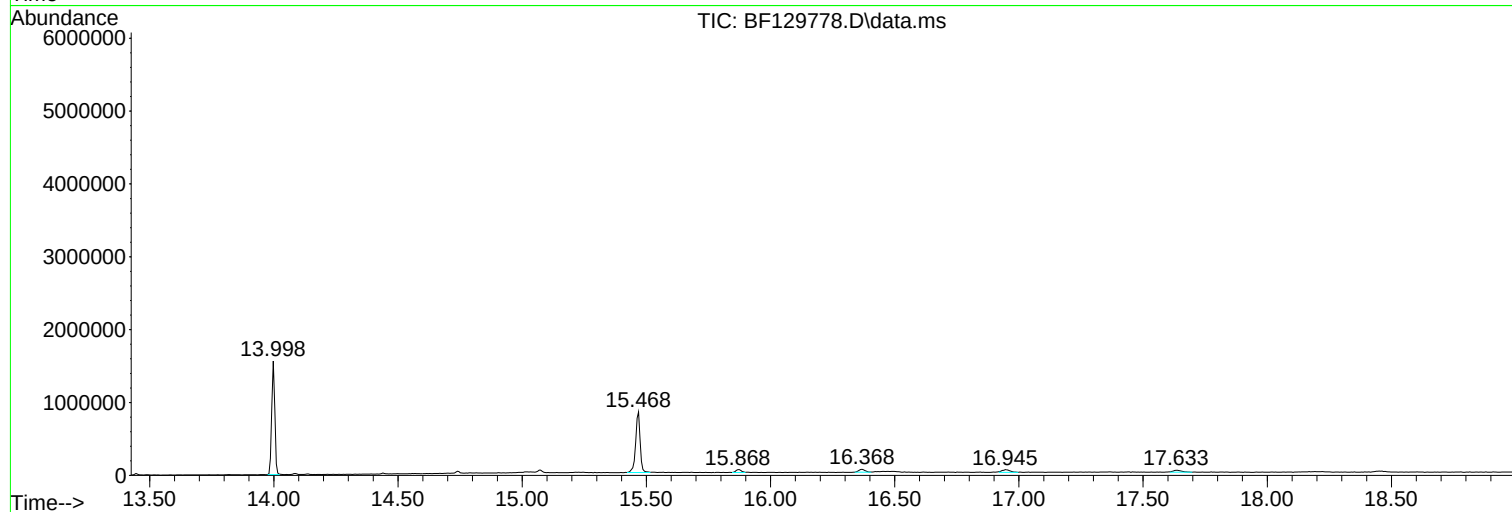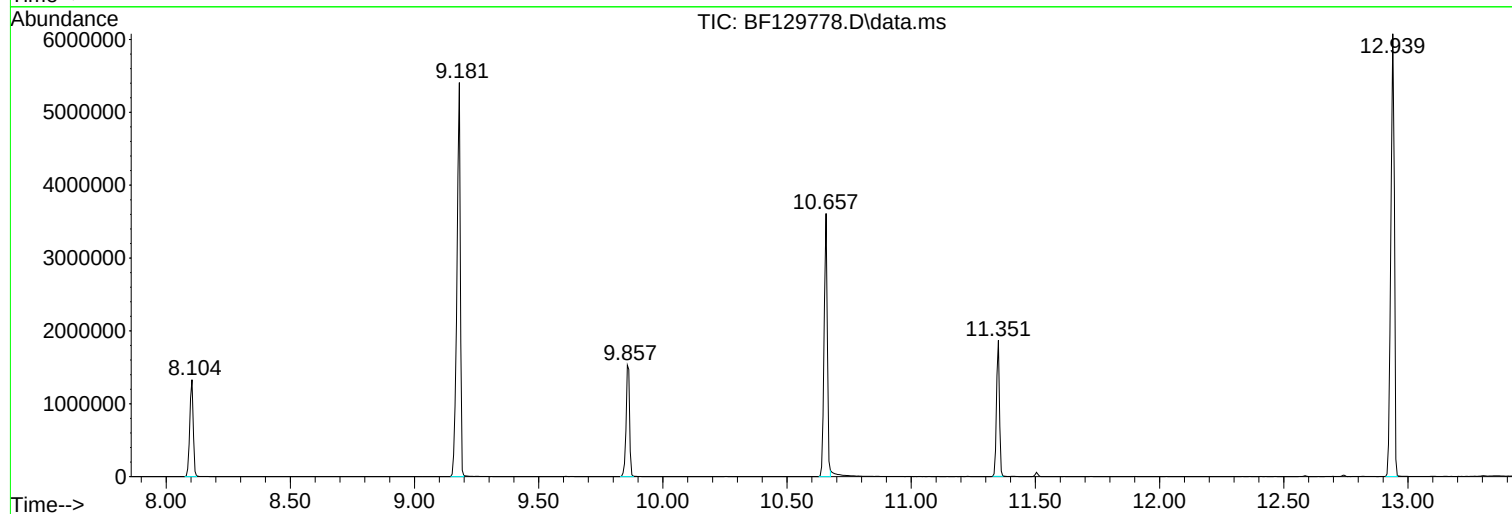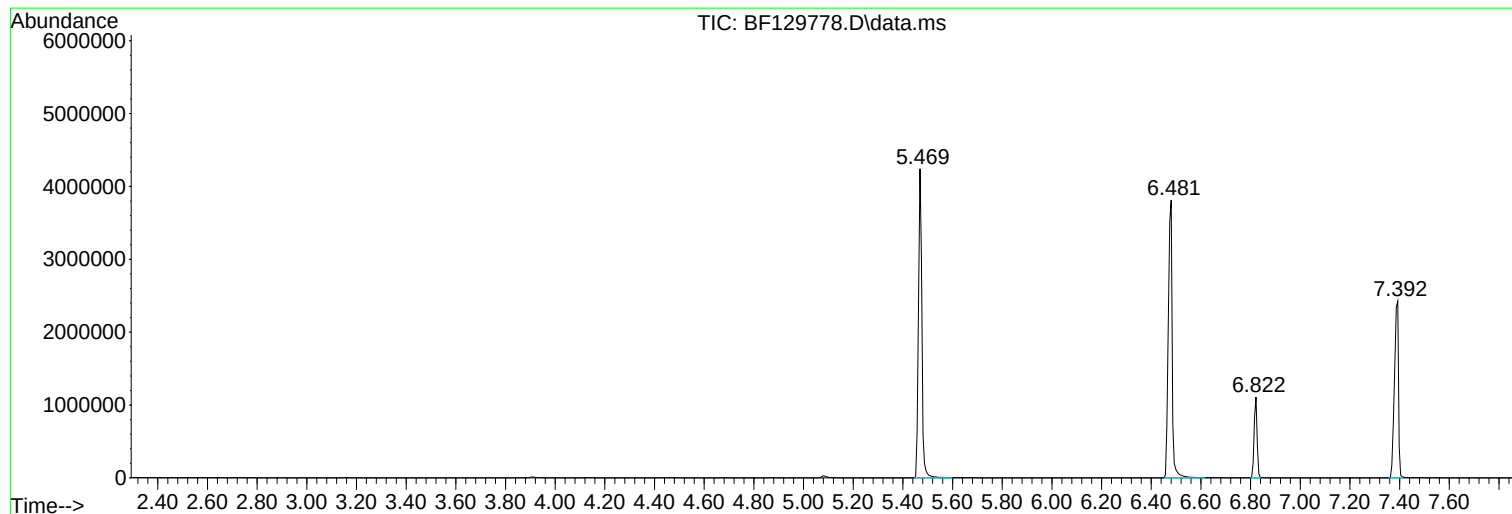

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129778.D
Acq On : 14 Aug 2022 23:32
Operator : CG\JU
Sample : PB146737BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129778.D
Acq On : 14 Aug 2022 23:32
Operator : CG\JU
Sample : PB146737BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146737BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------