


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
 Data File : BF129760.D
 Acq On : 14 Aug 2022 13:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 15 02:28:31 2022

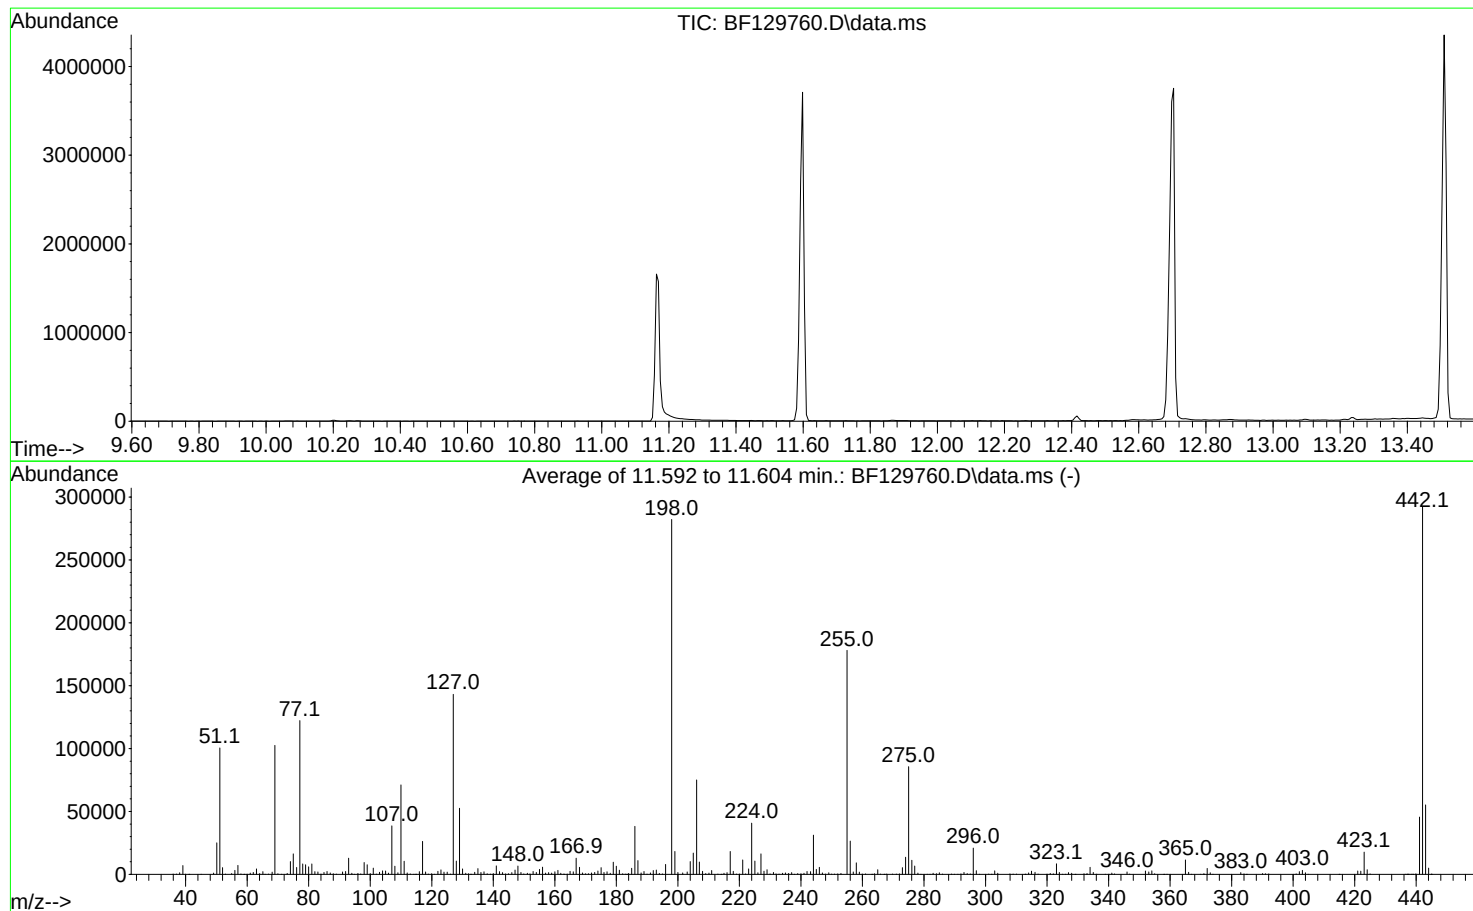


AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1576

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	100509	PASS
68	69	0.00	2	1.7	1775	PASS
69	198	0.00	100	36.3	102552	PASS
70	69	0.00	2	0.5	492	PASS
127	198	10	80	50.7	143139	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	282181	PASS
199	198	5	9	6.5	18262	PASS
275	198	10	60	30.4	85659	PASS
365	198	1	100	4.0	11419	PASS
441	198	0.01	100	16.1	45568	PASS
442	442	50	100	100.0	292459	PASS
443	442	15	24	18.9	55213	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
 Data File : BF129760.D
 Acq On : 14 Aug 2022 13:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 15 05:53:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 15 02:28:31 2022
 Response via : Initial Calibration

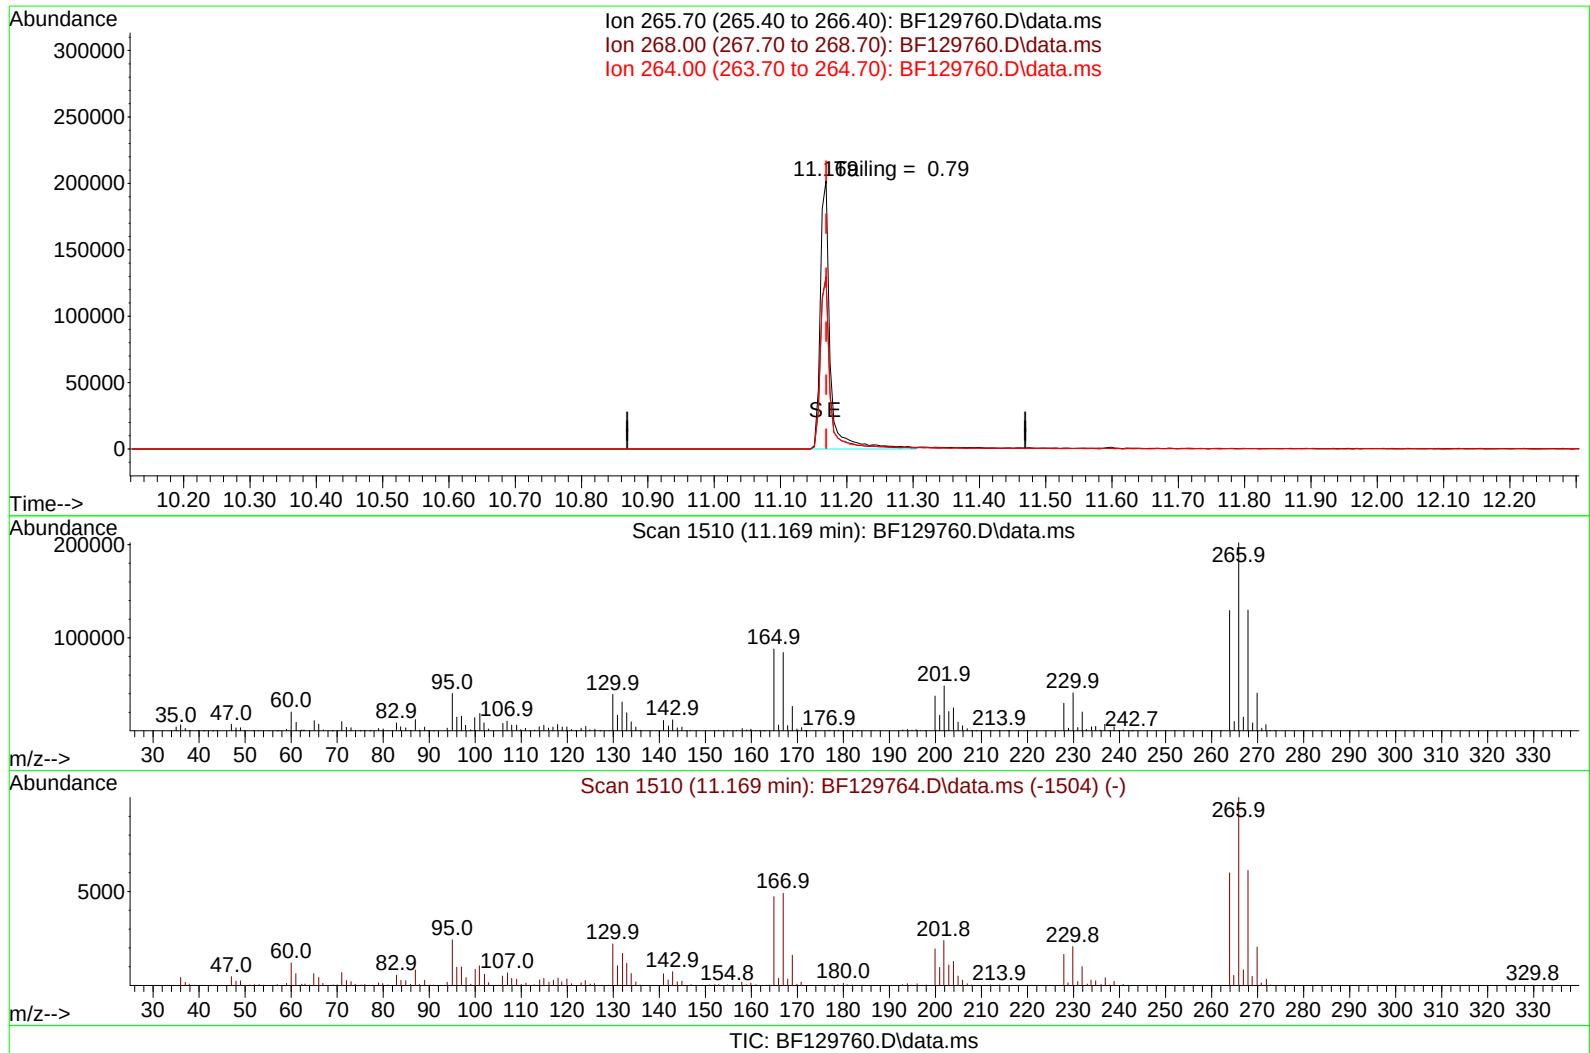

(70) Pentachlorophenol (C)

11.169min (-0.000) 106918.19 ng




response 210859

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.17
264.00	59.90	63.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081422\
Data File : BF129760.D
Acq On : 14 Aug 2022 13:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 05:53:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

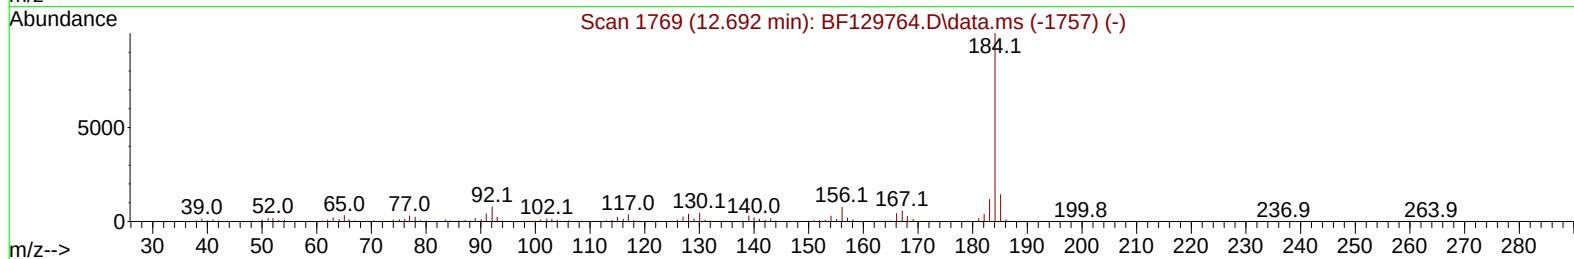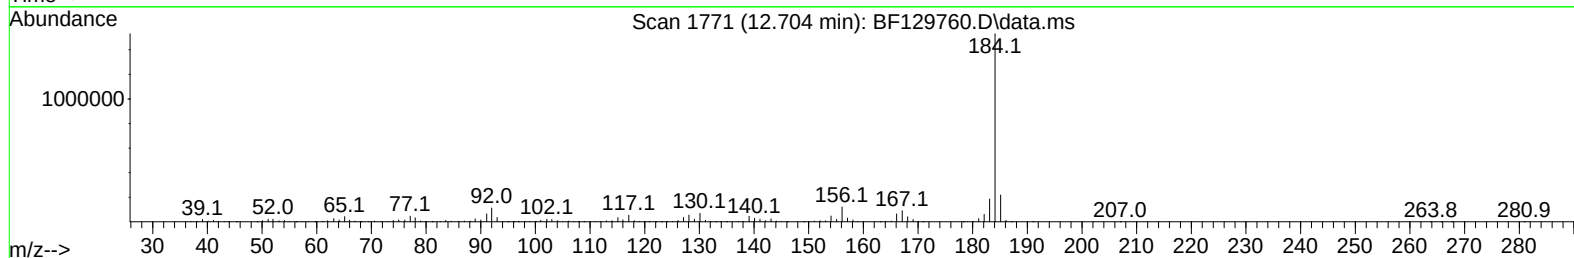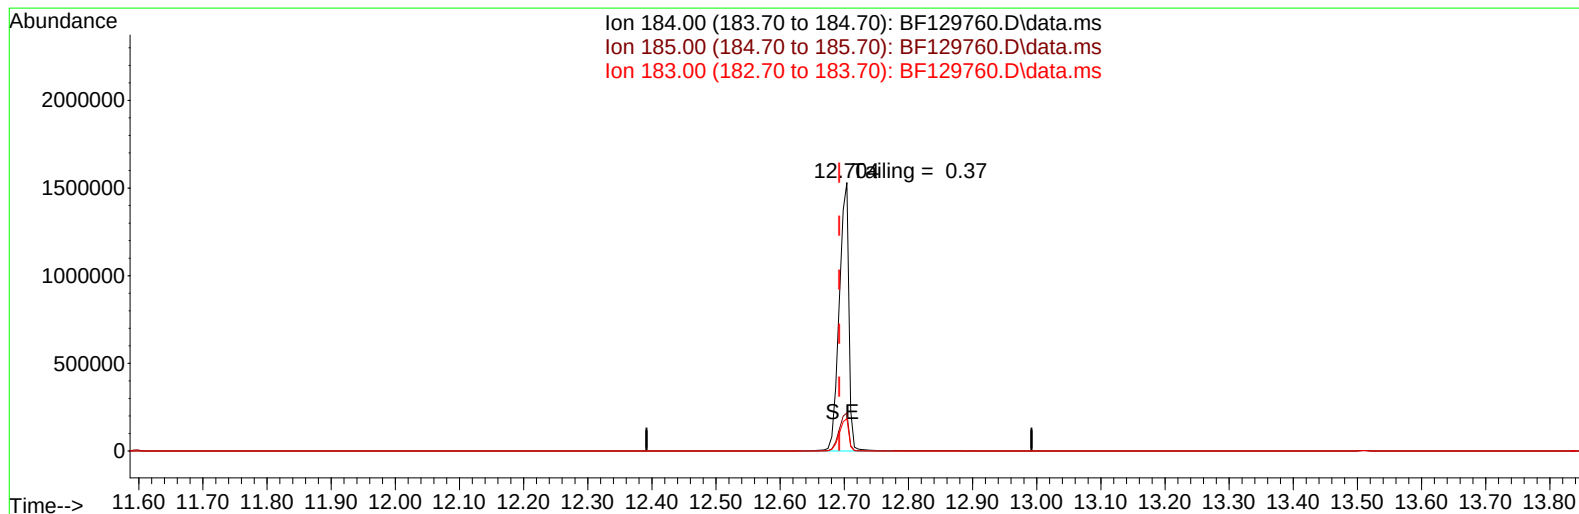

TIC: BF129760.D\data.ms

(77) Benzidine

12.704min (+ 0.012) 75643.92 ng

response 1610819

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.19
183.00	11.80	12.07
0.00	0.00	0.00

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/14/2022	BNA_F	<u>BF129760.D</u>
Compound Name	Response	Retention Time
DDT	757748	13.51
DDD	7243	13.233
DDE	1534	12.875
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8777	766525	1.15