
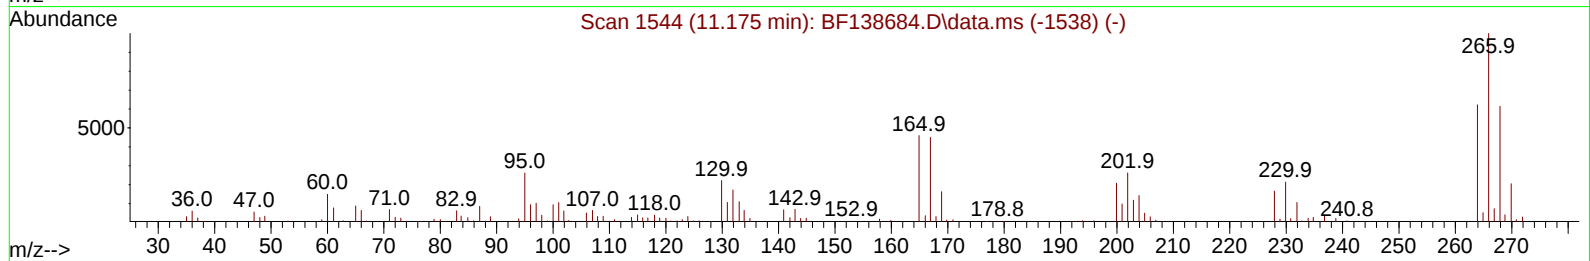
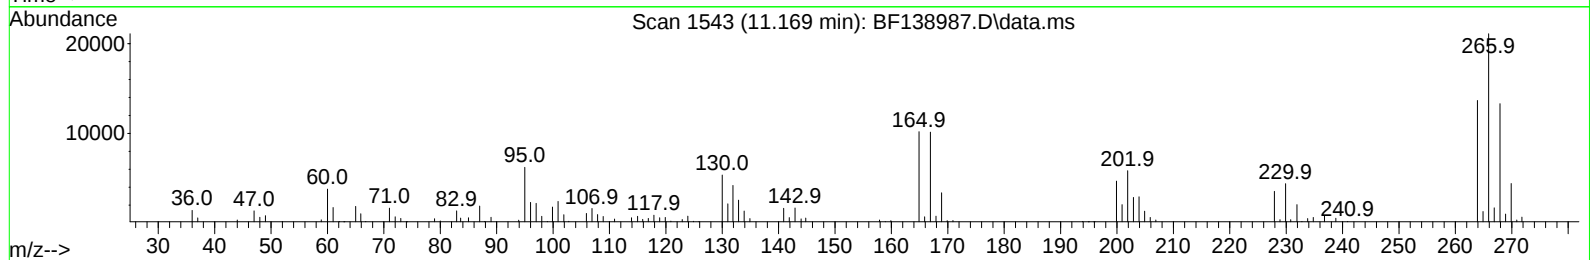


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
Data File : BF138987.D
Acq On : 14 Aug 2024 11:33
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 12:15:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

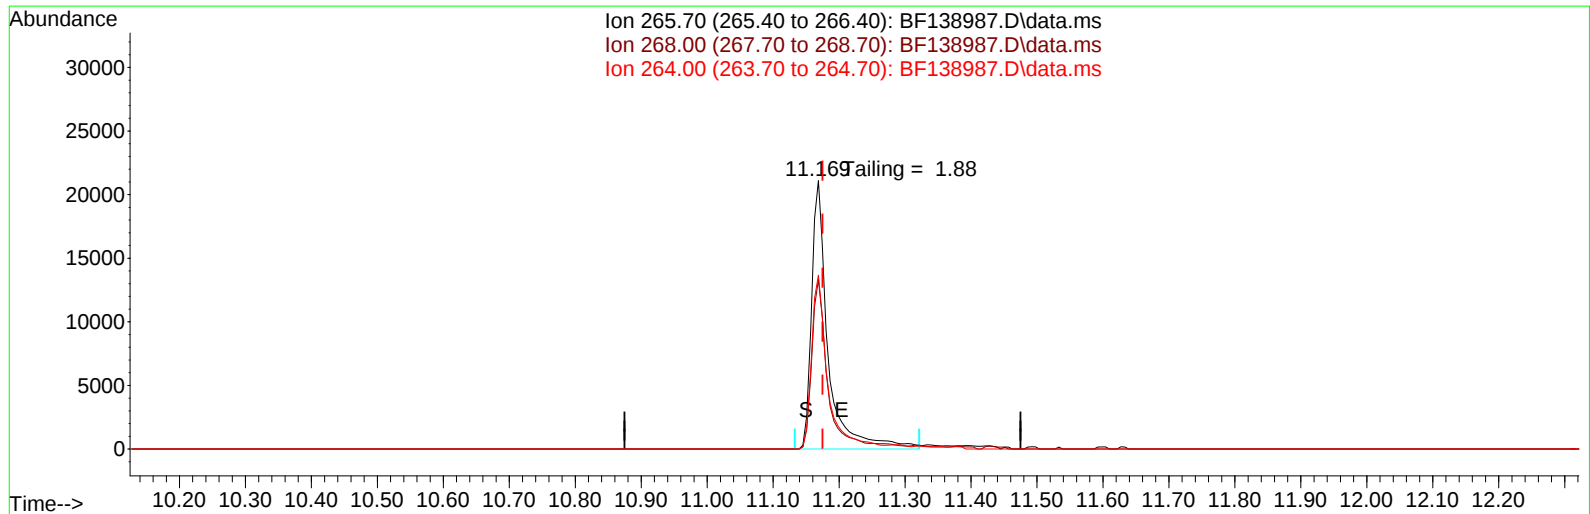

TIC: BF138987.D\data.ms




(70) Pentachlorophenol (C)

11.169min (-0.006) 42832.92 ng

response 37122

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.09
264.00	62.20	64.73
0.00	0.00	0.00

Quant Time: Aug 14 12:15:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

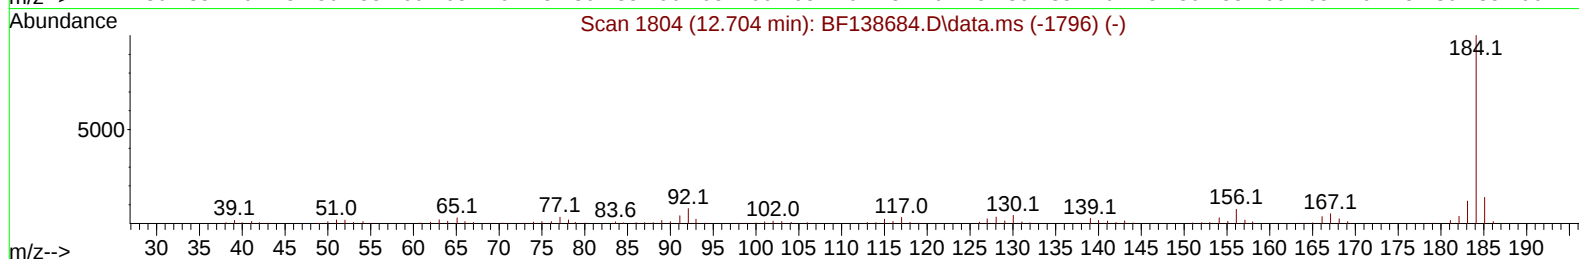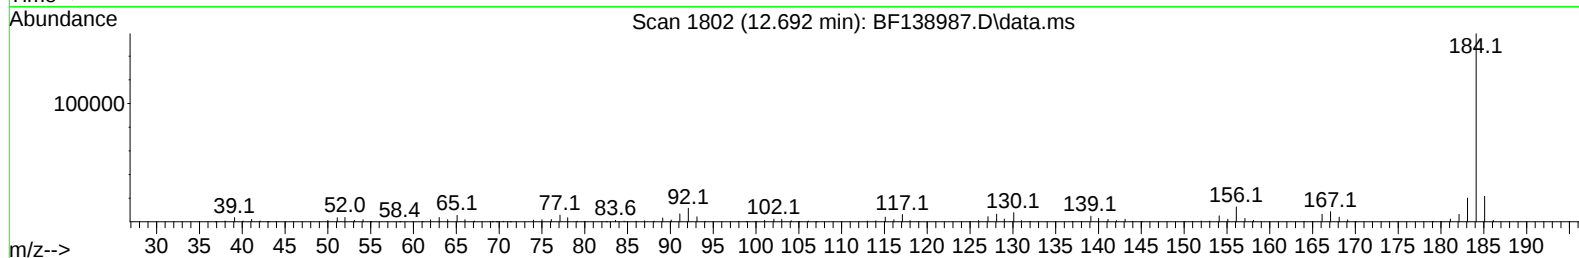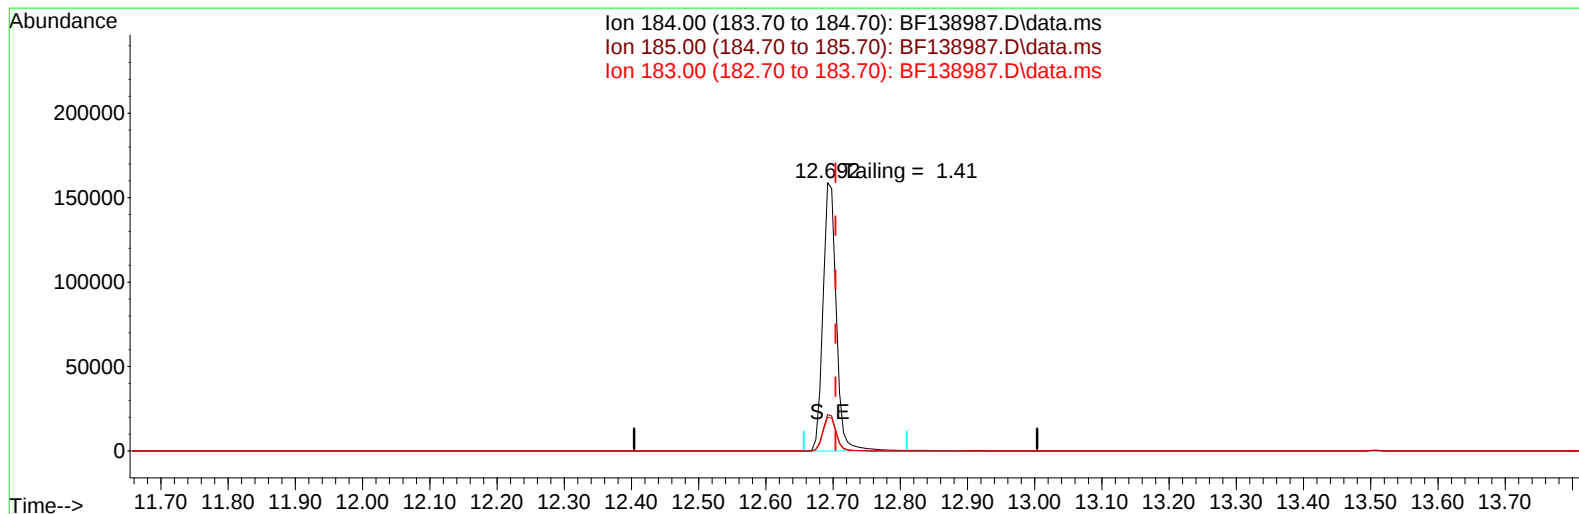

TIC: BF138987.D\data.ms

(77) Benzidine

12.692min (-0.012) 0.00 ng

response **218193**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.59
183.00	12.00	12.68
0.00	0.00	0.00