

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
 Data File : BF138994.D
 Acq On : 14 Aug 2024 15:09
 Operator : RC/JU
 Sample : P3512-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 931-K1-SD-0.5-1.0-080724-FD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	499	504	521	rBV	28518	44927	5.95%	0.901%
2	5.469	569	574	604	rBV	496316	709813	93.93%	14.232%
3	6.481	741	746	767	rBV	535260	755700	100.00%	15.152%
4	6.834	801	806	815	rVB	187349	227855	30.15%	4.569%
5	7.398	897	902	915	rBV	352519	460637	60.96%	9.236%
6	7.663	943	947	957	rBB2	5959	10595	1.40%	0.212%
7	8.116	1019	1024	1041	rBB	234086	290762	38.48%	5.830%
8	8.440	1075	1079	1091	rBV	13744	22064	2.92%	0.442%
9	9.187	1201	1206	1216	rBV	566504	699486	92.56%	14.025%
10	9.863	1316	1321	1331	rBV	251950	318063	42.09%	6.377%
11	9.957	1332	1337	1344	rVV	9211	12644	1.67%	0.254%
12	10.657	1451	1456	1470	rBV	277707	363954	48.16%	7.298%
13	11.351	1569	1574	1584	rBV	210759	271912	35.98%	5.452%
14	12.933	1838	1843	1848	rBV	362287	439387	58.14%	8.810%
15	13.998	2019	2024	2035	rVB	127298	171974	22.76%	3.448%
16	14.439	2093	2099	2104	rBV2	5590	8739	1.16%	0.175%
17	15.074	2202	2207	2212	rBV	10689	14274	1.89%	0.286%
18	15.457	2266	2272	2283	rVB	92080	151294	20.02%	3.034%
19	15.868	2336	2342	2349	rBV	7248	13259	1.75%	0.266%




Sum of corrected areas: 4987339

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
Data File : BF138994.D
Acq On : 14 Aug 2024 15:09
Operator : RC/JU
Sample : P3512-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
931-K1-SD-0.5-1.0-080724-FD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

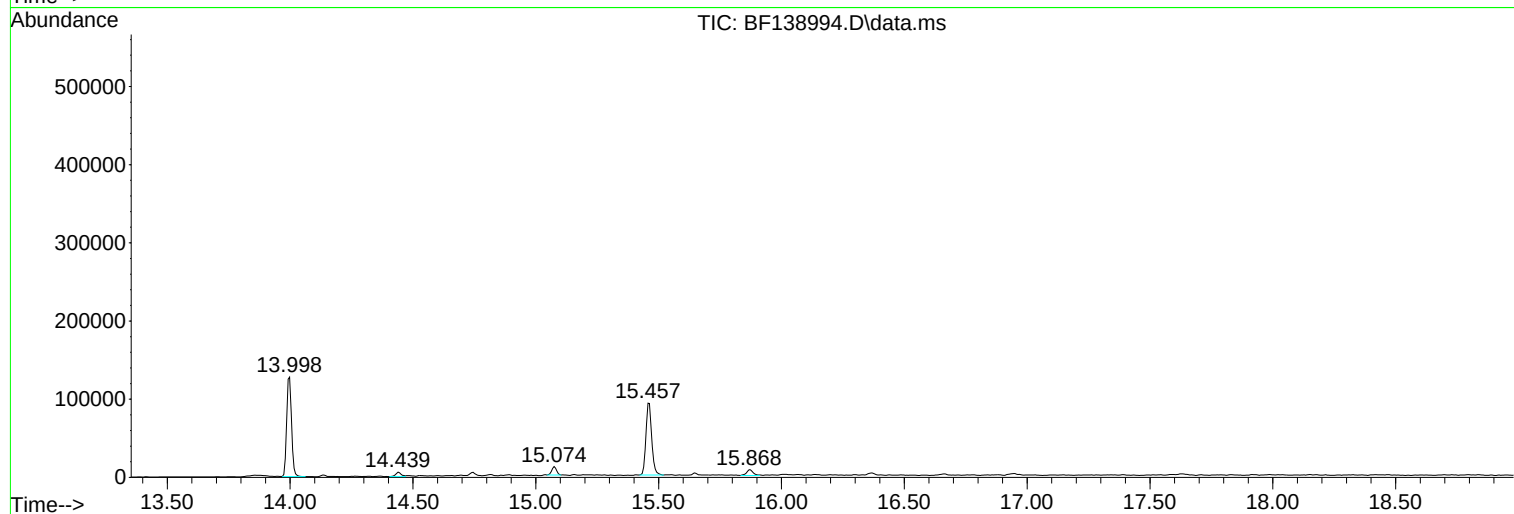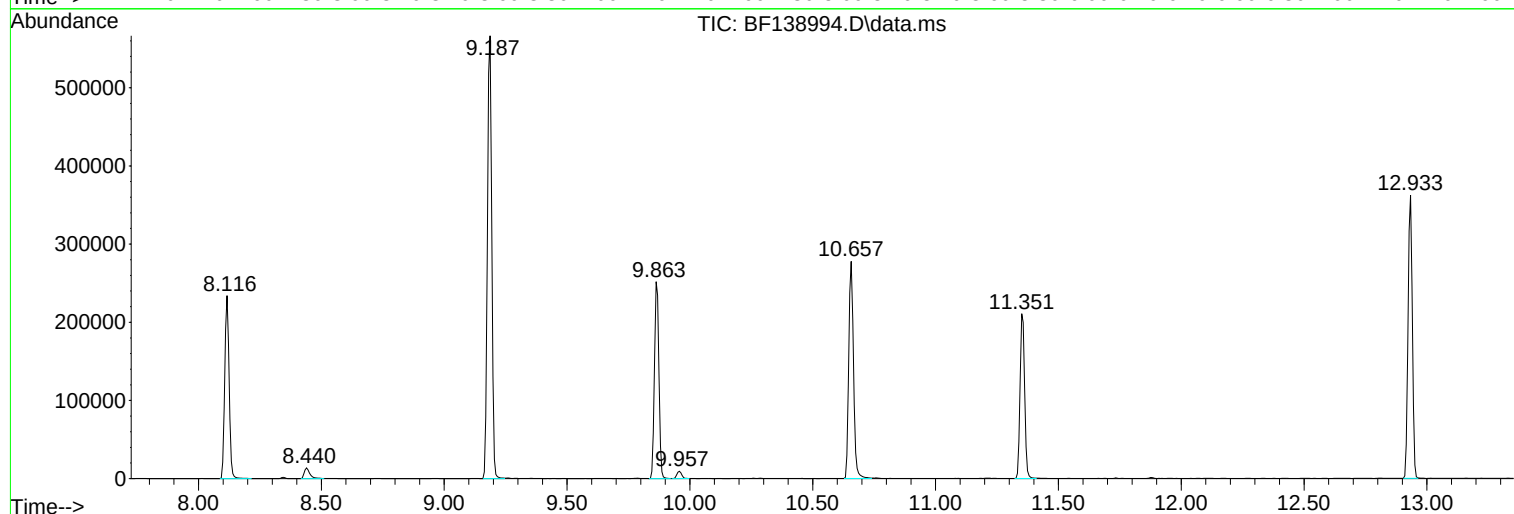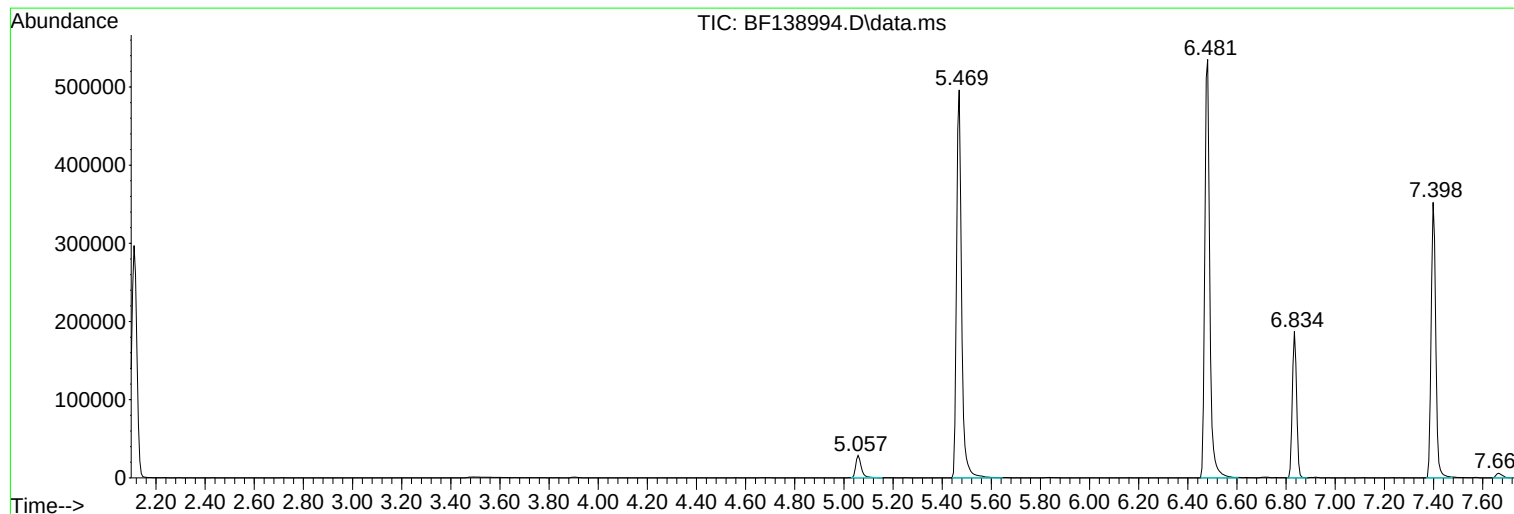

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
Data File : BF138994.D
Acq On : 14 Aug 2024 15:09
Operator : RC/JU
Sample : P3512-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
931-K1-SD-0.5-1.0-080724-FD










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.057	3.94 ng	44927	1,4-Dichlorobenzene-d4	6.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	3-Octanol	130	C8H18O	000589-98-0	36		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	Diacetamide	101	C4H7NO2	000625-77-4	9		

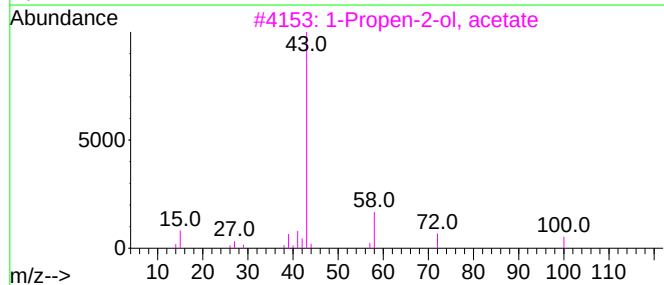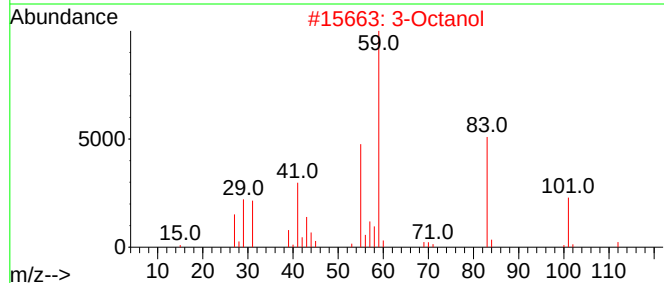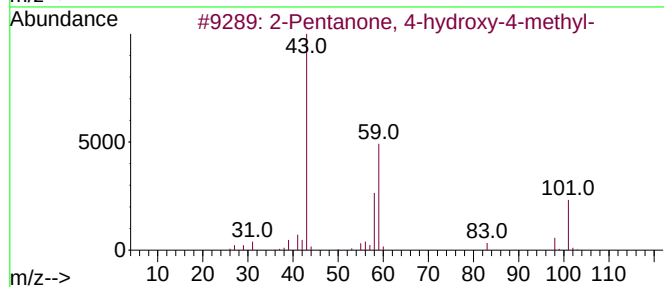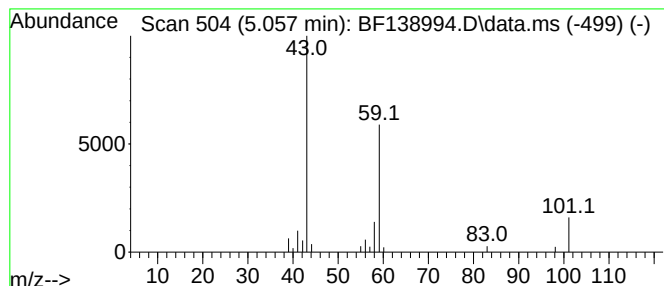

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081424\
Data File : BF138994.D
Acq On : 14 Aug 2024 15:09
Operator : RC/JU
Sample : P3512-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
931-K1-SD-0.5-1.0-080724-FD

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.057	3.9	ng	44927	1	6.834	227855	20.0