


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081424\  
Data File : BF138987.D  
Acq On : 14 Aug 2024 11:33  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Jul 30 17:50:01 2024

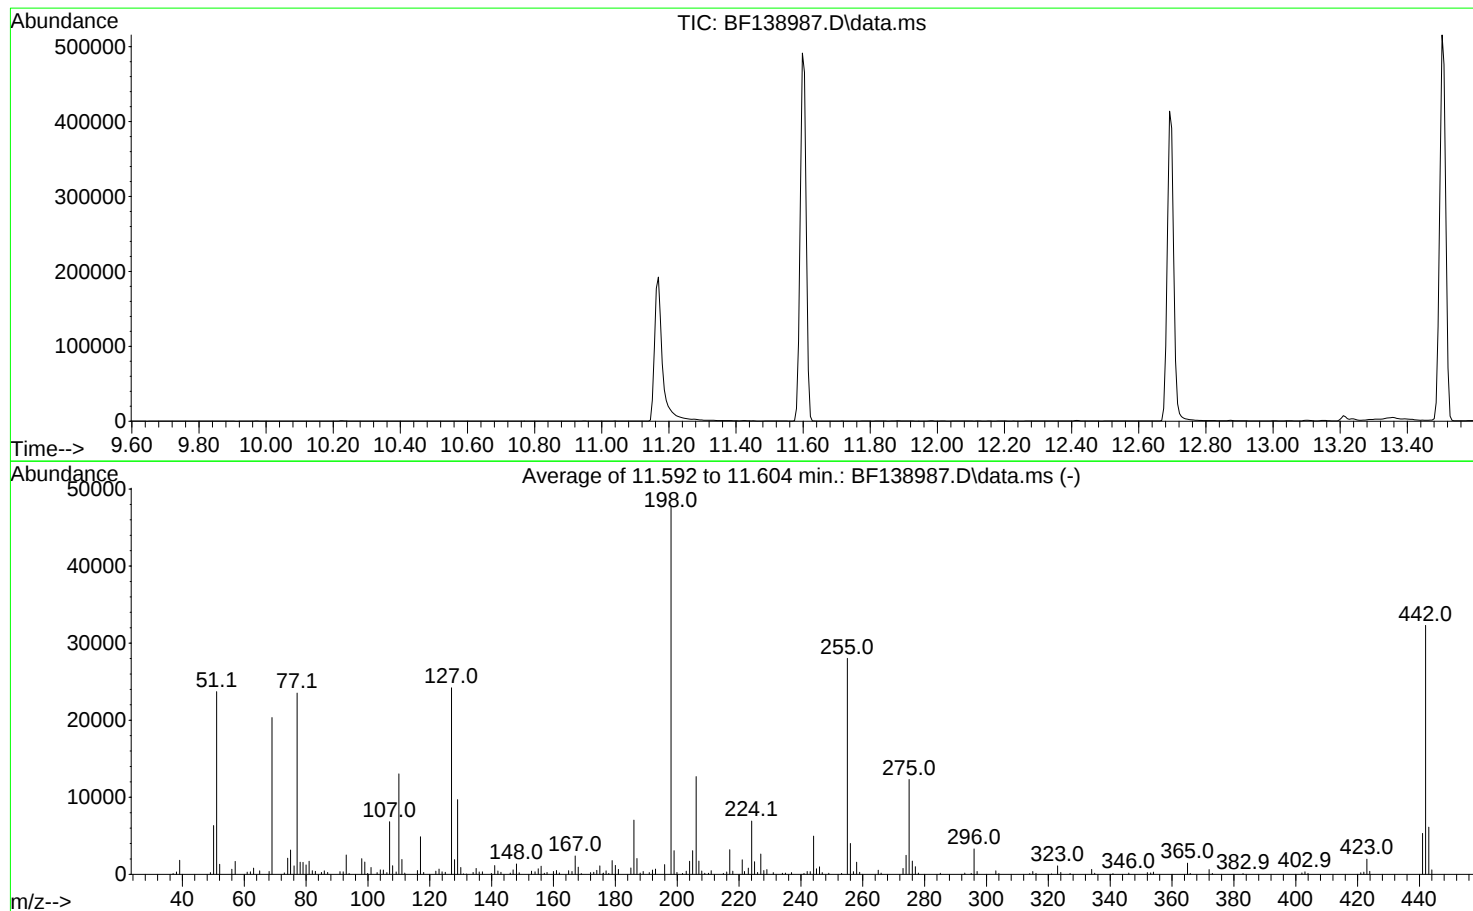

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 49.7         | 23707      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 376        | PASS                |
| 69             | 198             | 0.00            | 100             | 42.6         | 20352      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 50.7         | 24208      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 47733      | PASS                |
| 199            | 198             | 5               | 9               | 6.4          | 3077       | PASS                |
| 275            | 198             | 10              | 60              | 25.8         | 12322      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 1447       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.1         | 5317       | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 32304      | PASS                |
| 443            | 442             | 15              | 24              | 18.9         | 6121       | PASS                |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/14/2024     | BNA_F            | <u>BF138987.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 122337           | 13.504             |
| DDD           | 3496             | 13.21              |
| DDE           | 243              | 12.874             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3739          | 126076           | 2.97               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081424\  
Data File : BF138987.D  
Acq On : 14 Aug 2024 11:33  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 14 12:15:04 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 30 17:50:01 2024  
Response via : Initial Calibration

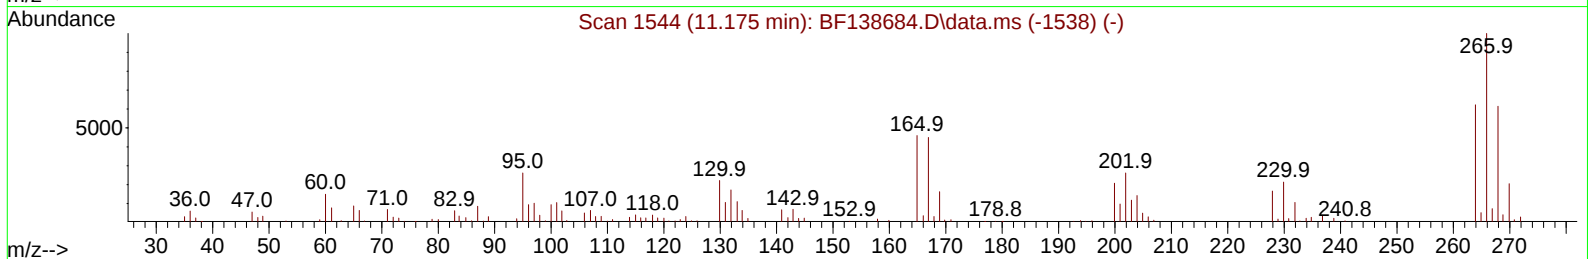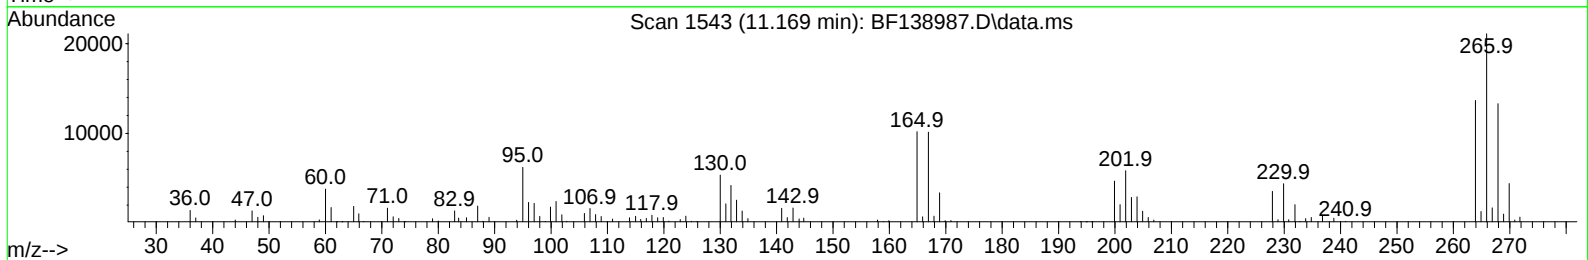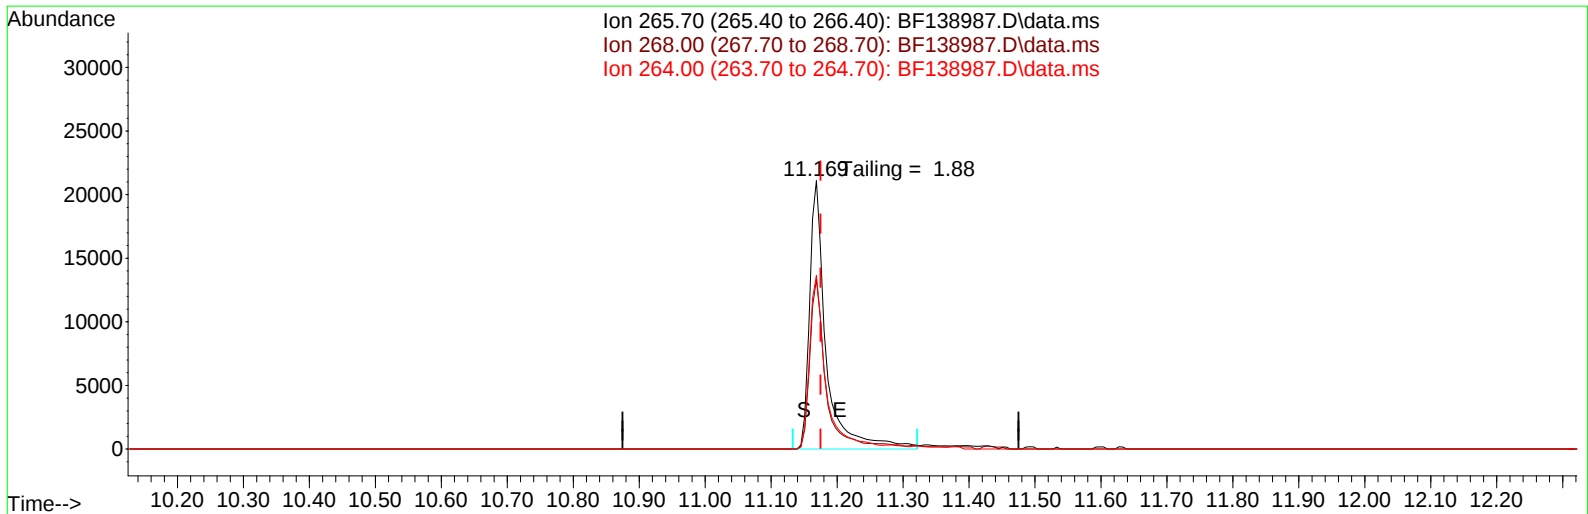

TIC: BF138987.D\data.ms

**(70) Pentachlorophenol (C)**

**11.169min (-0.006) 42832.92 ng**




**response 37122**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.50  | 63.09  |
| 264.00 | 62.20  | 64.73  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081424\  
Data File : BF138987.D  
Acq On : 14 Aug 2024 11:33  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 14 12:15:04 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF073024.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 30 17:50:01 2024  
Response via : Initial Calibration

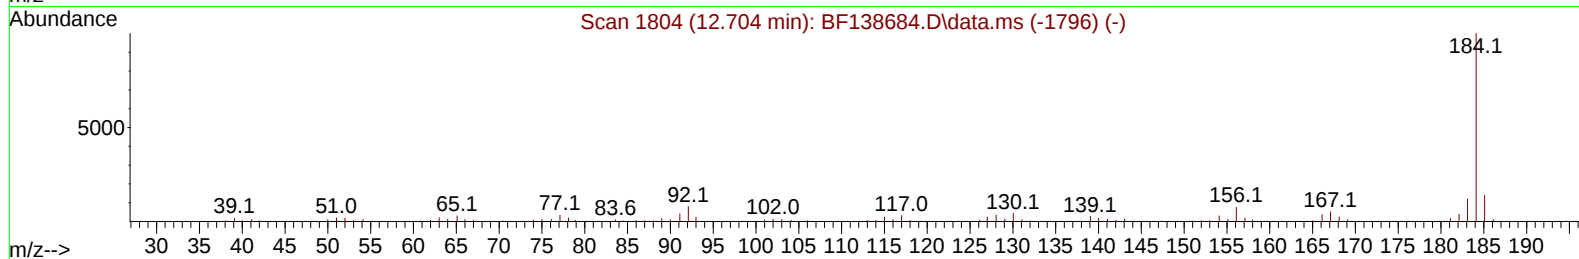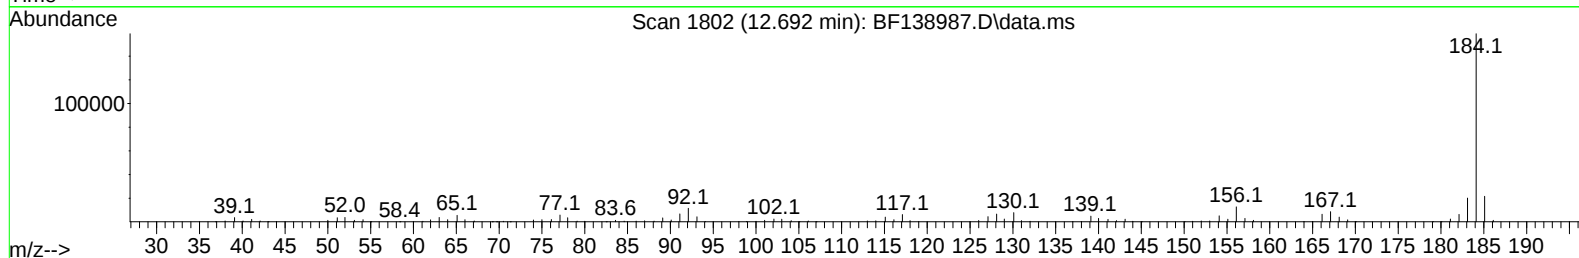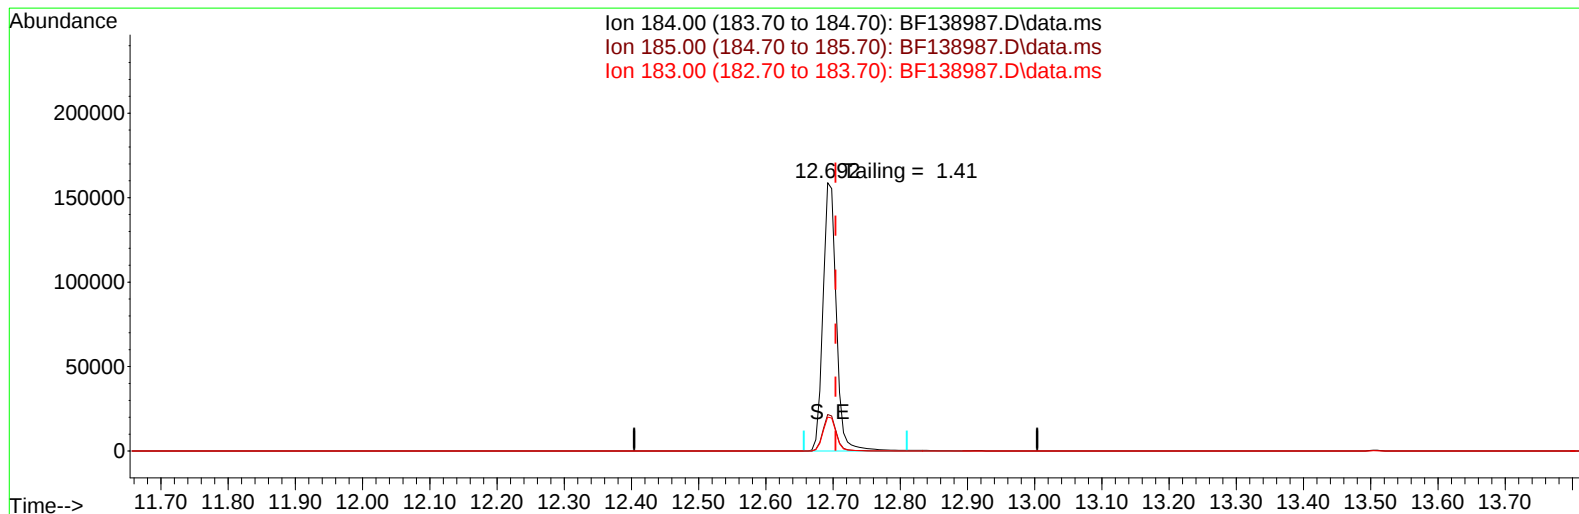

TIC: BF138987.D\data.ms

(77) Benzidine

12.692min (-0.012) 0.00 ng

response 218193

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.90  | 13.59  |
| 183.00 | 12.00  | 12.68  |
| 0.00   | 0.00   | 0.00   |