
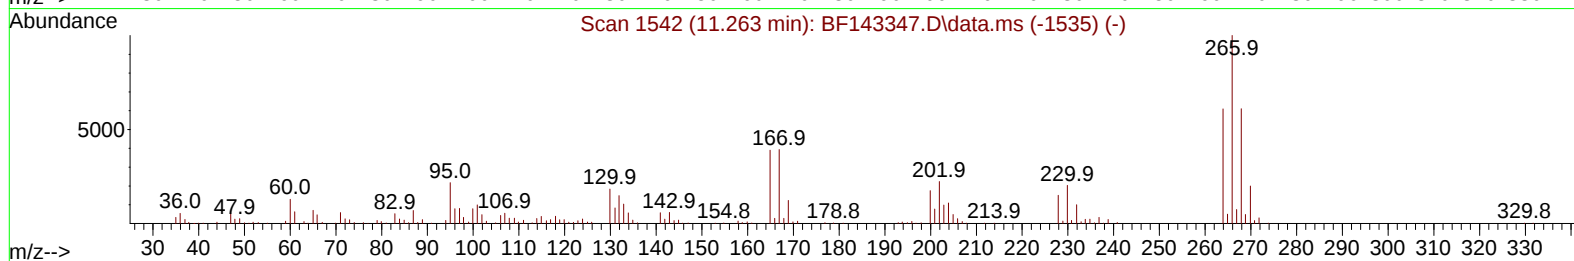
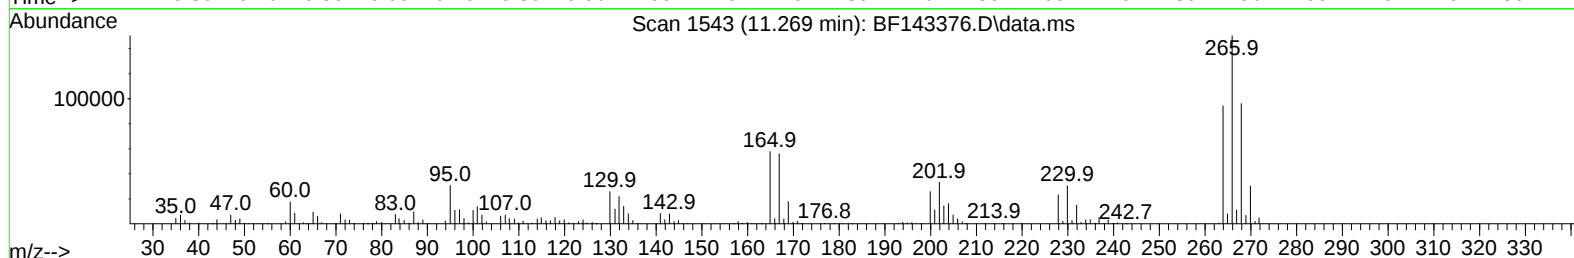


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143376.D
Acq On : 14 Aug 2025 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 12:58:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

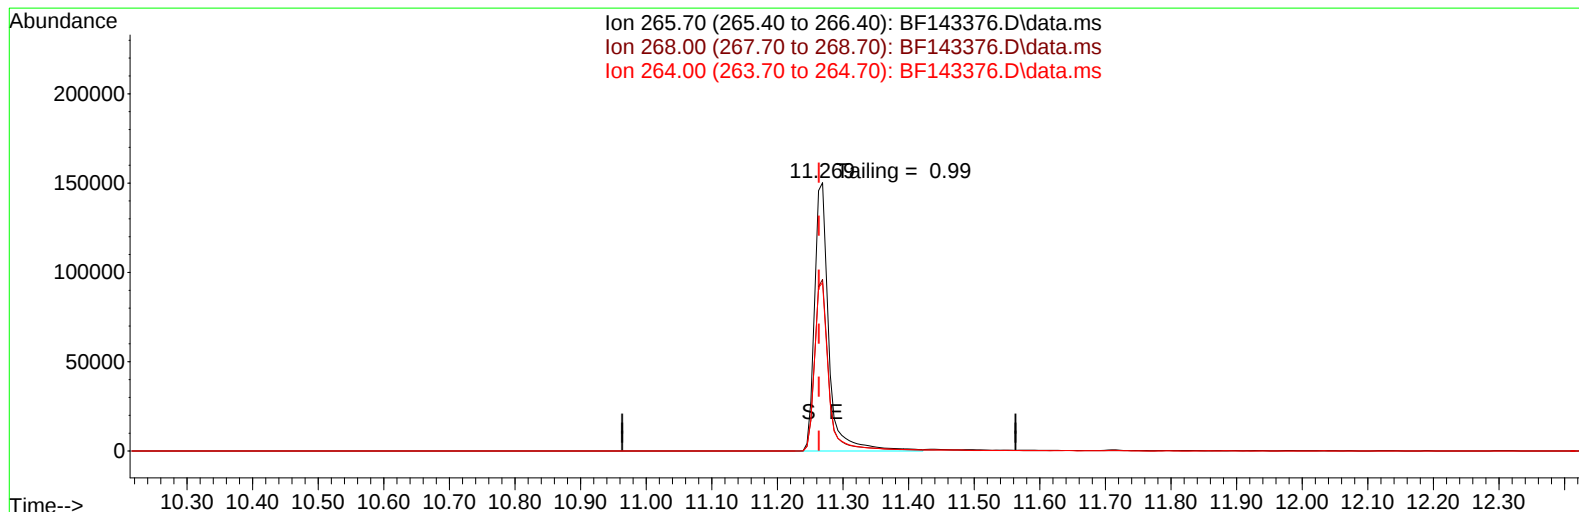

TIC: BF143376.D\data.ms

(70) Pentachlorophenol (C)




11.269min (+ 0.006) 295541.56 ng

response 227255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.95
264.00	61.00	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143376.D
Acq On : 14 Aug 2025 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 12:58:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

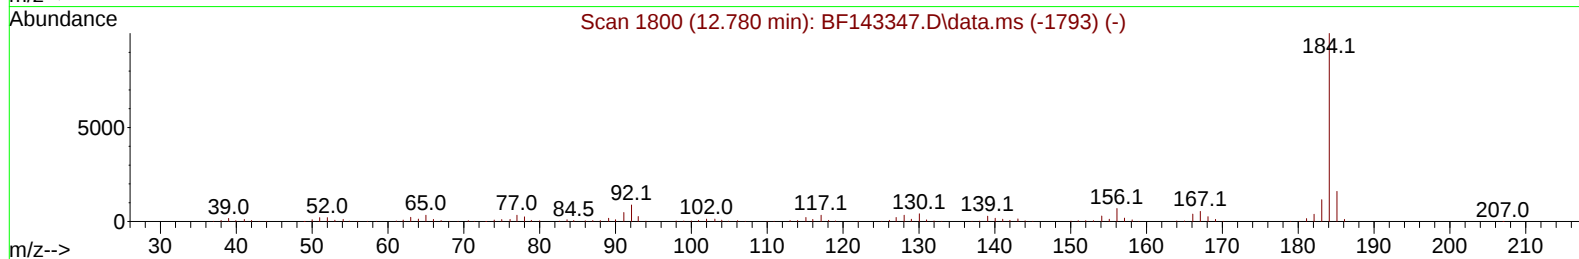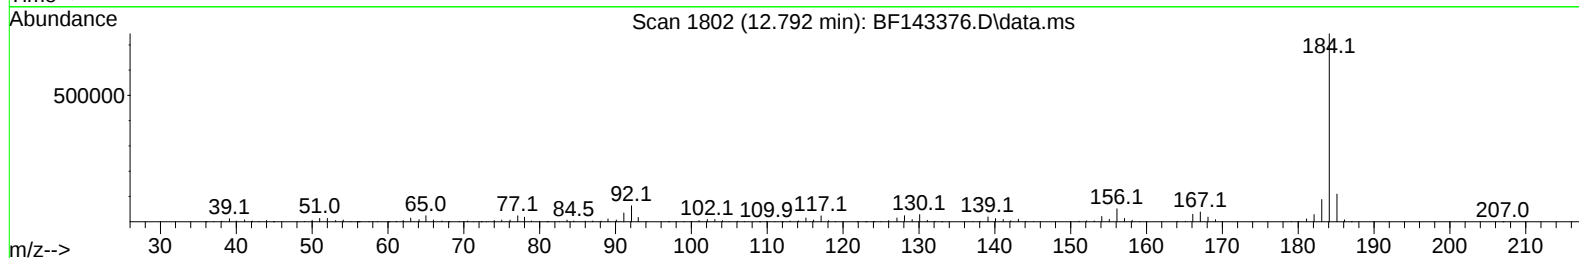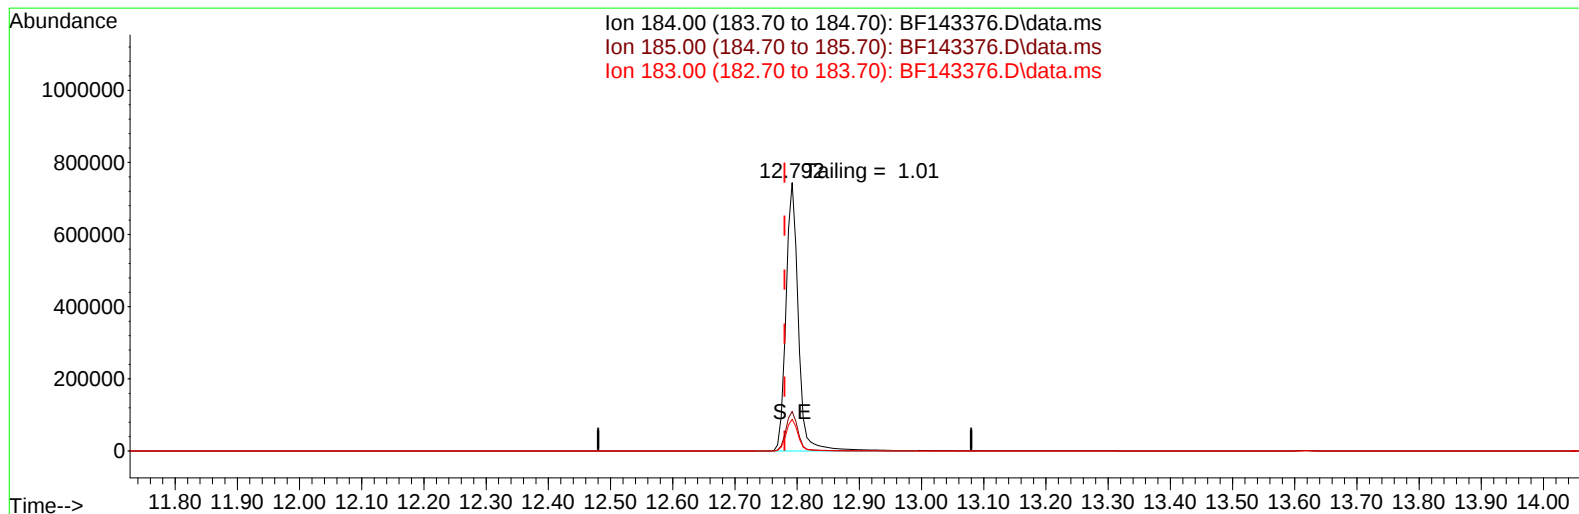

TIC: BF143376.D\data.ms

(77) Benzidine

12.792min (+ 0.012) 0.00 ng

response 1039955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.73
183.00	11.60	11.82
0.00	0.00	0.00