
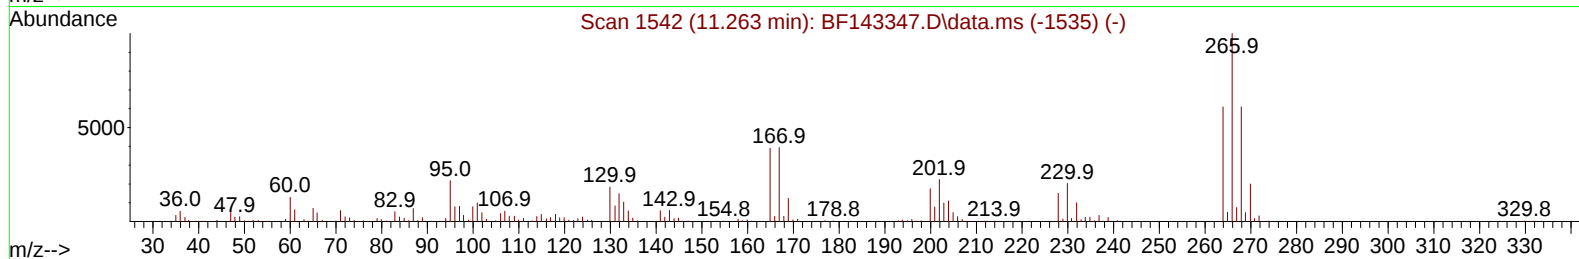
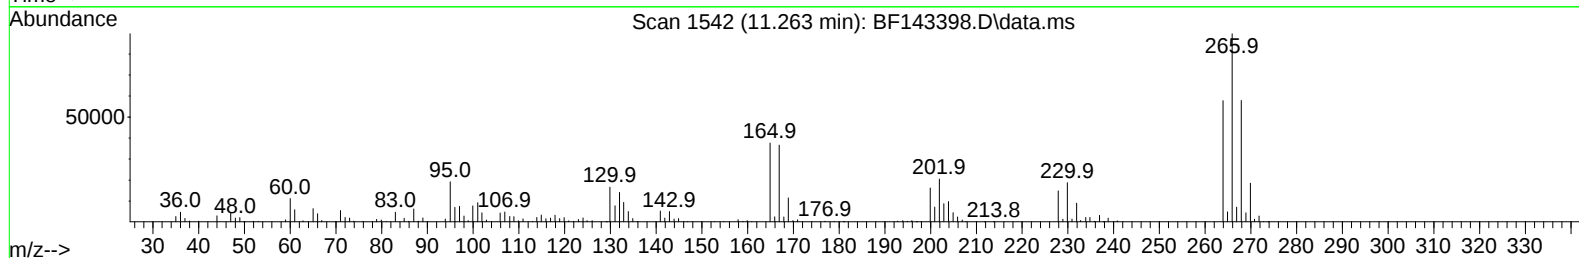


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143398.D
Acq On : 15 Aug 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 03:37:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

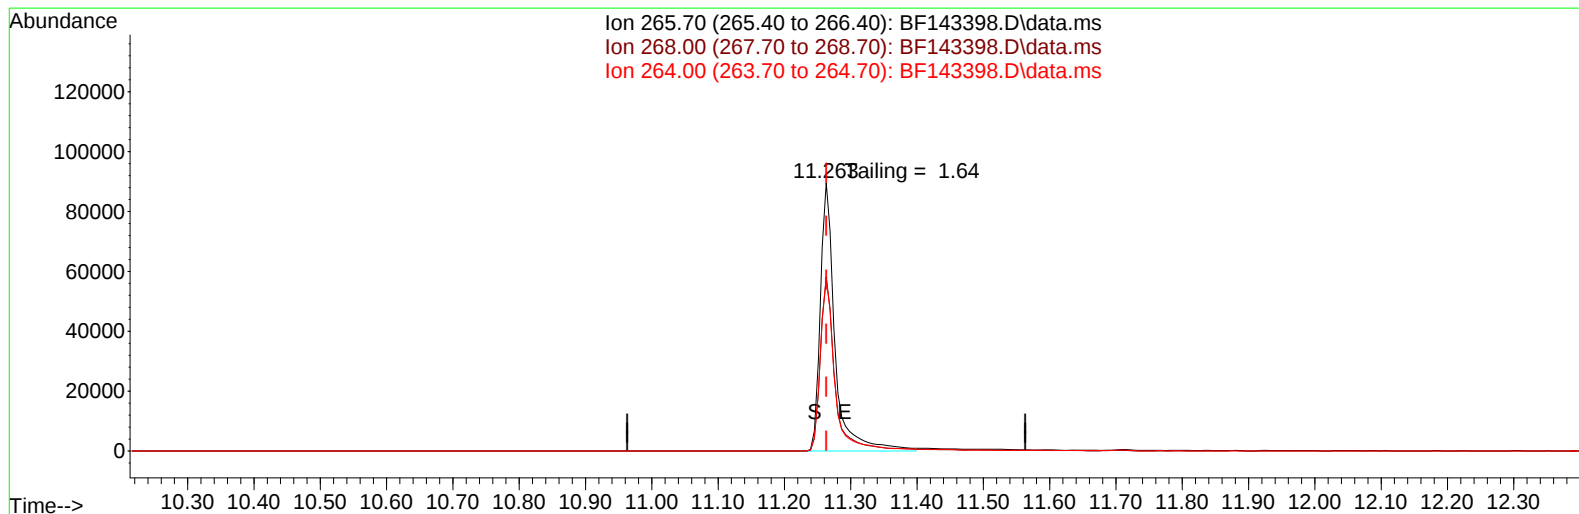

TIC: BF143398.D\data.ms

(70) Pentachlorophenol (C)




11.263min (-0.000) 83327.89 ng

response 139002

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.61
264.00	61.00	64.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143398.D
Acq On : 15 Aug 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 03:37:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

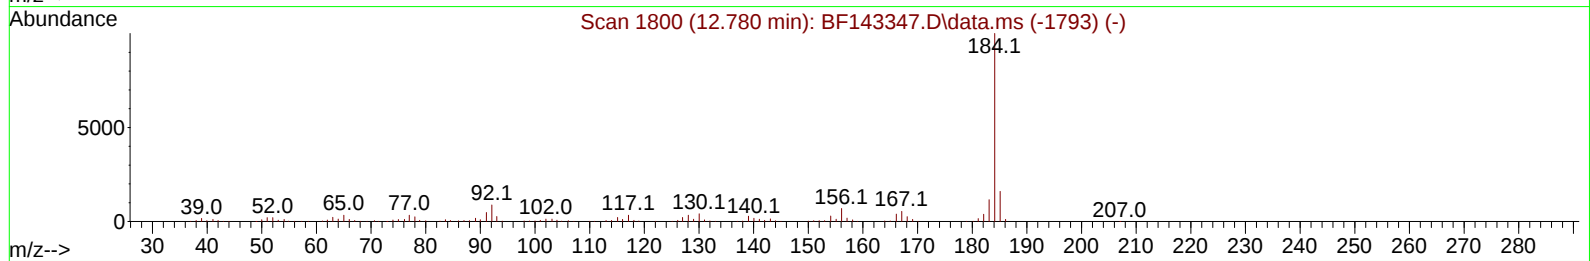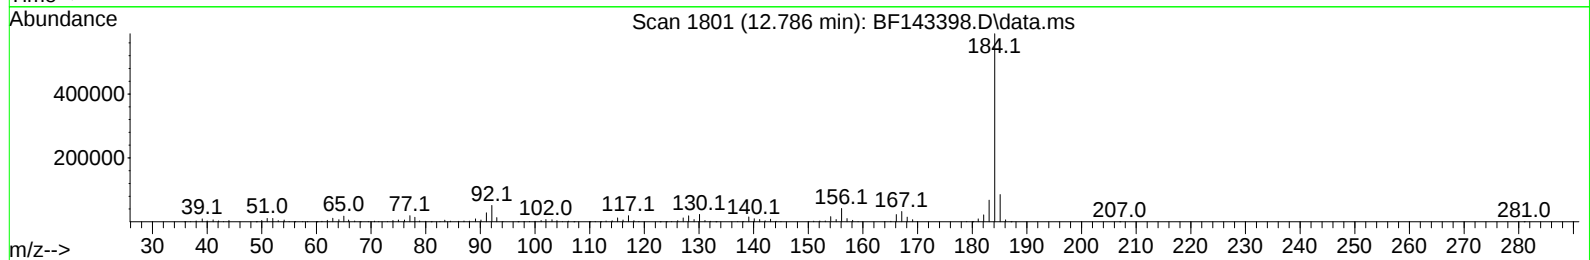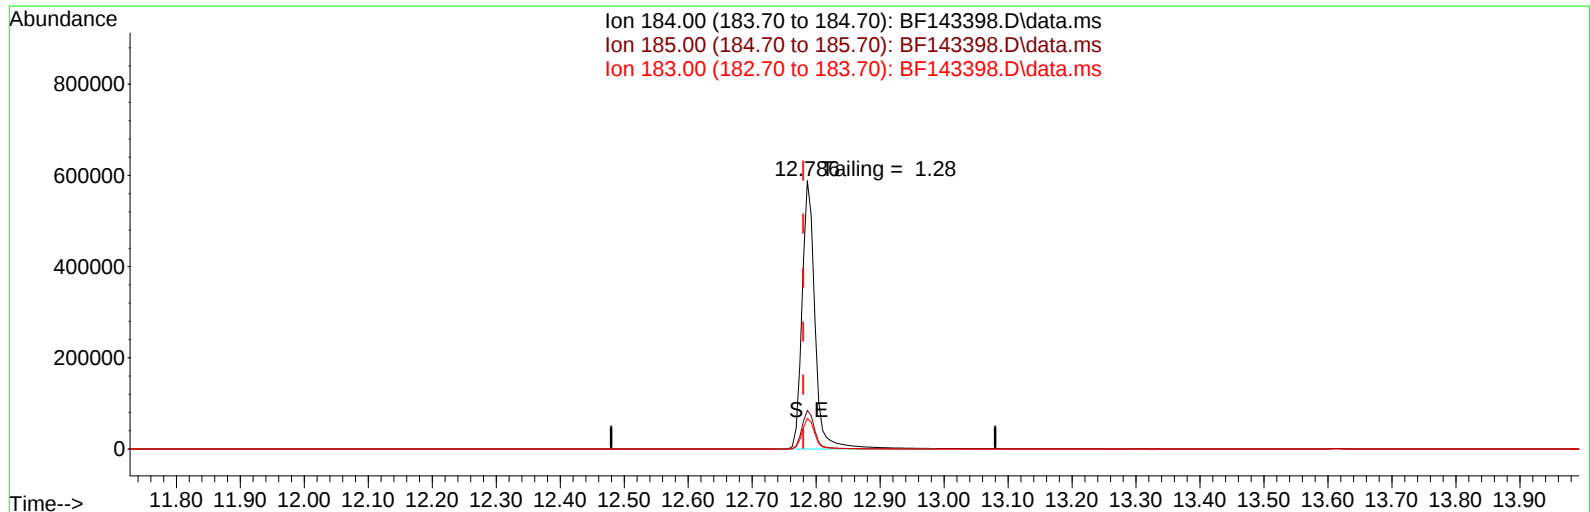

TIC: BF143398.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 830815

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.46
183.00	11.60	11.48
0.00	0.00	0.00