
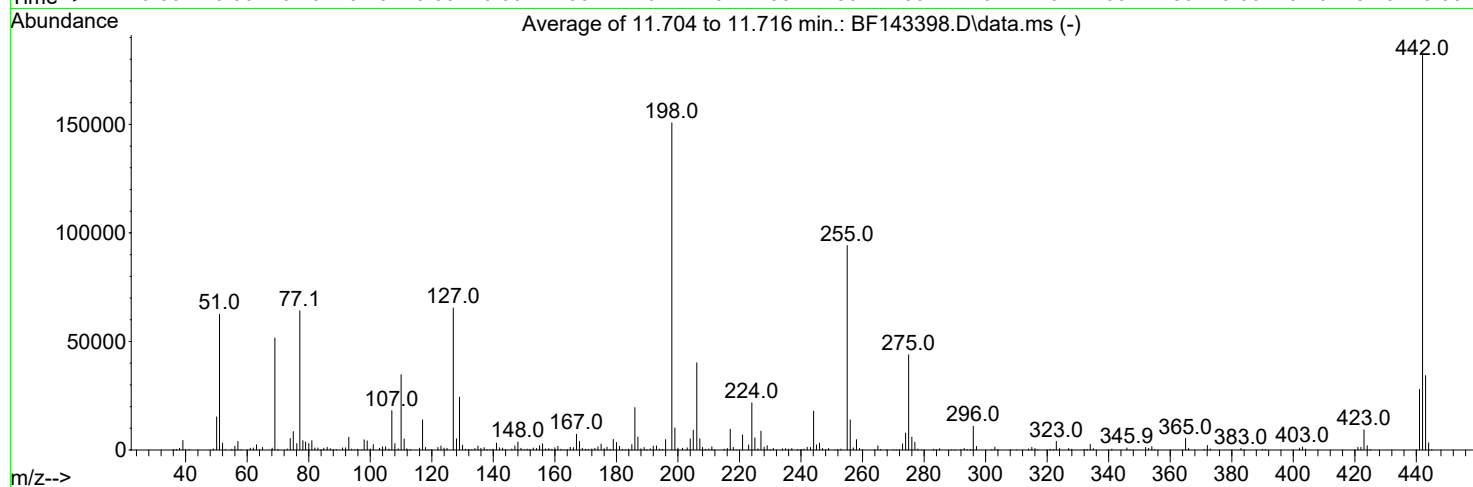


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143398.D
Acq On : 15 Aug 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 12 13:25:39 2025

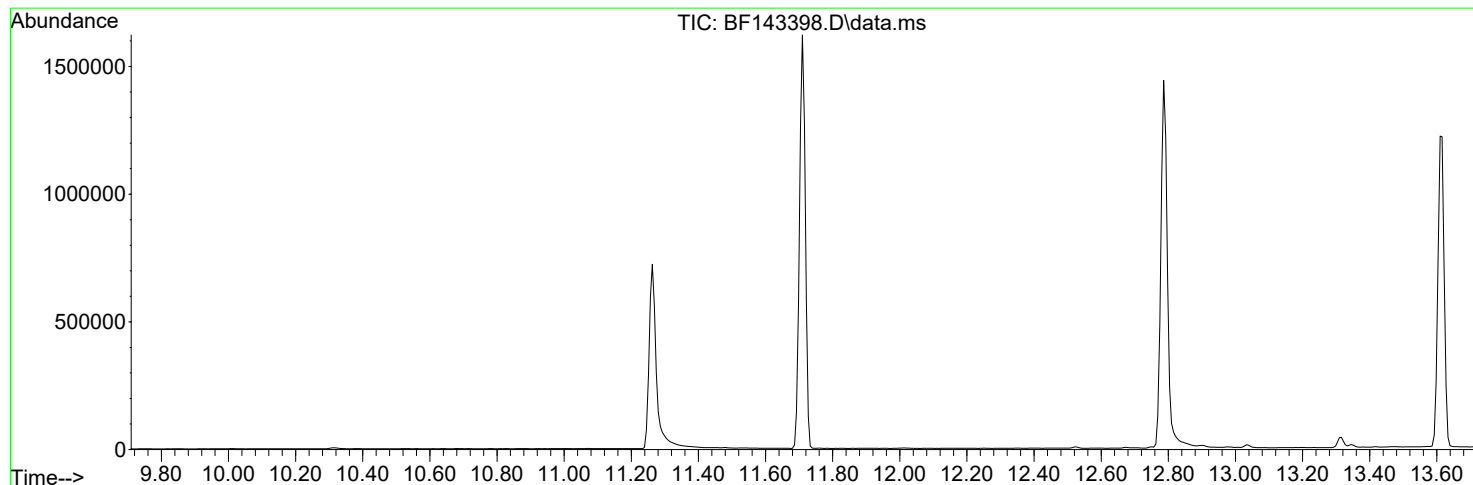

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.7	886	PASS
69	69	100	100	100.0	51568	PASS
70	69	0.00	2	0.6	319	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	150741	PASS
199	198	5	9	6.8	10206	PASS
365	198	1	100	3.6	5358	PASS
441	443	0.01	150	81.5	27955	PASS
442	442	100	100	100.0	181899	PASS
443	442	15	24	18.8	34285	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/14/2025	BNA_F	<u>BF143398.D</u>
Compound Name	Response	Retention Time
DDT	317573	13.619
DDD	15212	13.316
DDE	914	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16126	333699	4.83

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143398.D
Acq On : 15 Aug 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 03:37:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

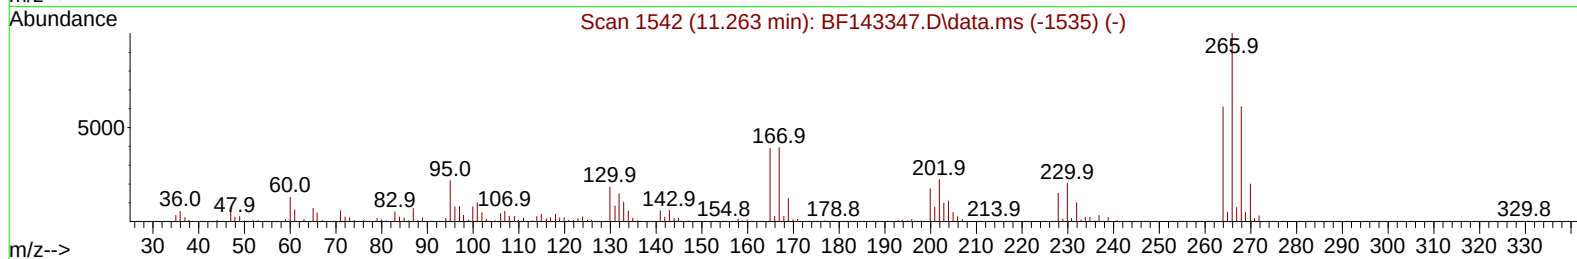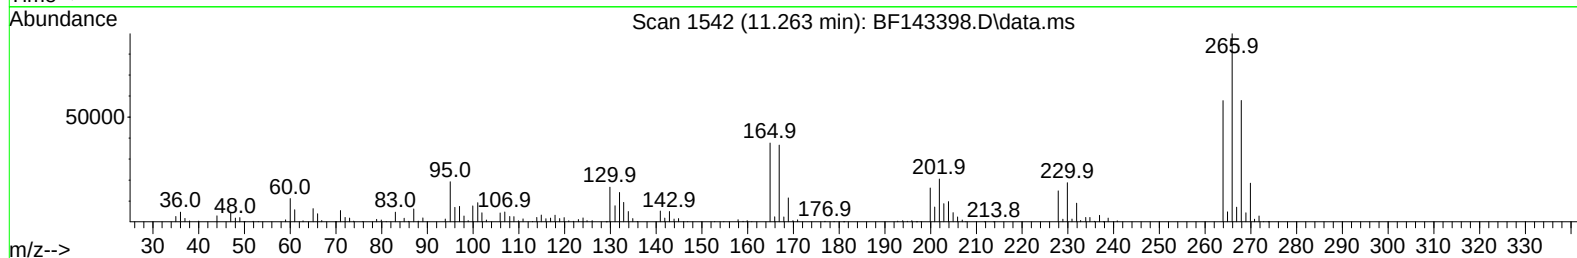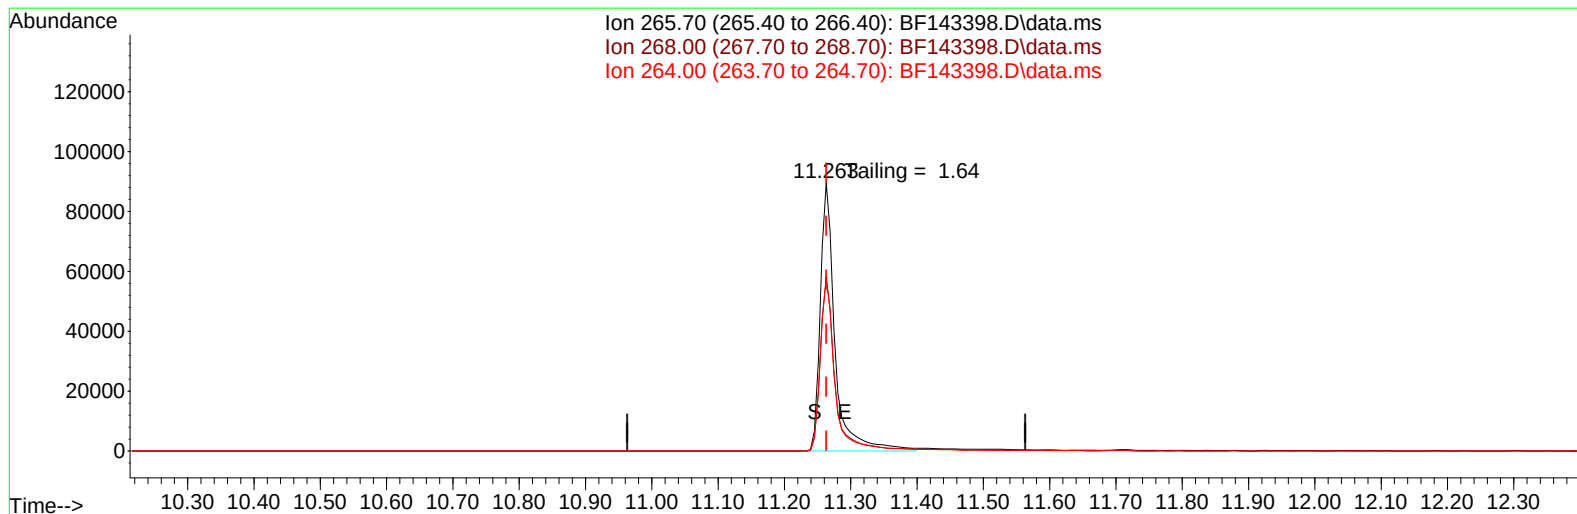

TIC: BF143398.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.000) 83327.89 ng




response 139002

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.61
264.00	61.00	64.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143398.D
Acq On : 15 Aug 2025 01:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 03:37:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

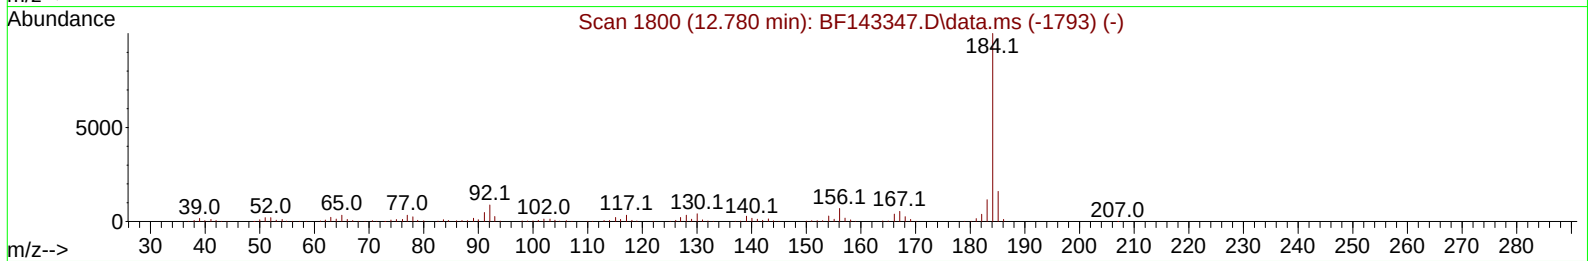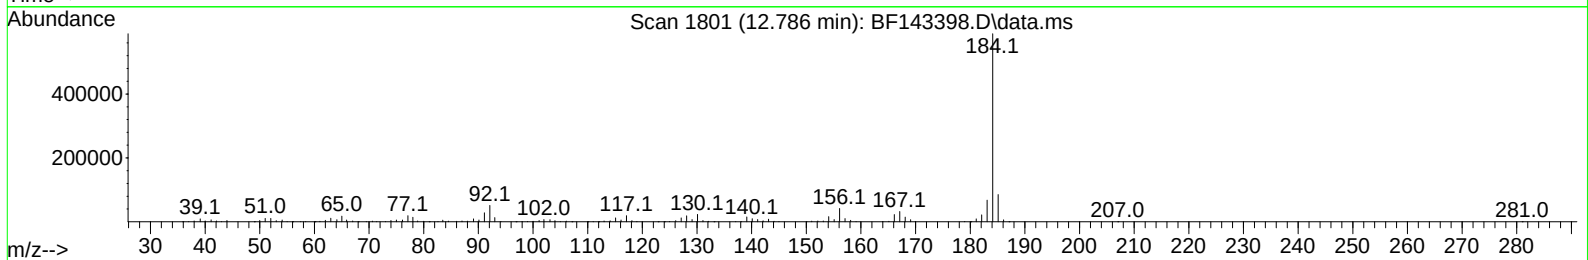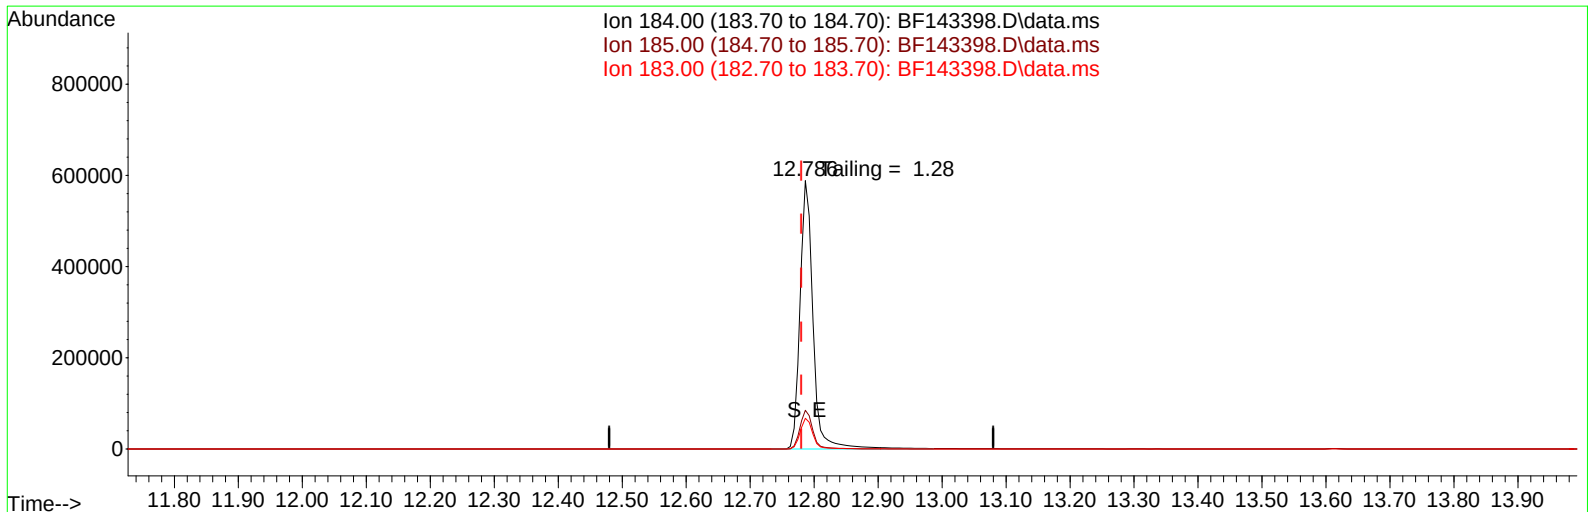

TIC: BF143398.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 830815

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.46
183.00	11.60	11.48
0.00	0.00	0.00