

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081517\
 Data File : BF097732.D
 Acq On : 16 Aug 2017 11:04
 Operator : SJ/JU
 Sample : I4751-10DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-23-COMPDL

Quant Time: Aug 16 12:16:30 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 13:25:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	125957	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	479726	20.00	ng	0.00
38) Acenaphthene-d10	9.82	164	187131	20.00	ng	0.00
63) Phenanthrene-d10	11.30	188	277710	20.00	ng	0.00
75) Chrysene-d12	13.94	240	264079	20.00	ng	0.00
86) Perylene-d12	15.37	264	206614	20.00	ng	0.01

System Monitoring Compounds

5) 2-Fluorophenol	5.38	112	100444	12.13	ng	0.00
7) Phenol-d6	6.40	99	159008	14.13	ng	-0.01
23) Nitrobenzene-d5	7.34	82	87595	9.92	ng	-0.01
41) 2,4,6-Tribromophenol	10.60	330	9609	5.92	ng	0.00
44) 2-Fluorobiphenyl	9.14	172	126266	9.91	ng	0.00
78) Terphenyl-d14	12.89	244	75137	5.93	ng	0.00

Target Compounds


						Qvalue
25) Isophorone	7.34	82	87438	4.762	ng	# 67
32) Benzoic acid	7.85	122	144	6.427	ng	# 1
50) 2,6-Dinitrotoluene	9.82	165	24387	8.932	ng	# 34
51) Acenaphthene	9.85	154	35804	2.867	ng	98
55) 4-Nitrophenol	10.02	139	10085	3.589	ng	# 28
56) 2,4-Dinitrotoluene	9.82	165	24387	7.117	ng	# 34
57) Fluorene	10.36	166	37457	2.895	ng	98
70) Phenanthrene	11.33	178	500968	33.853	ng	99
71) Anthracene	11.37	178	109689	7.308	ng	98
72) Carbazole	11.53	167	39035	2.740	ng	99
74) Fluoranthene	12.52	202	686845	44.467	ng	99
77) Pyrene	12.74	202	651727	30.174	ng	98
80) Benzo(a)anthracene	13.93	228	336894	21.286	ng	96
82) Chrysene	13.96	228	300465	19.084	ng	97
85) Indeno(1,2,3-cd)pyrene	16.77	276	102465	8.847	ng	# 90
87) Benzo(b)fluoranthene	14.96	252	427100	32.794	ng	99
88) Benzo(k)fluoranthene	15.06	252	46246	3.780	ng	96
89) Benzo(a)pyrene	15.31	252	218429	18.945	ng	97
90) Dibenzo(a,h)anthracene	16.94	278	20059	2.137	ng	94
91) Benzo(g,h,i)perylene	17.19	276	93694	9.567	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081517\
Data File : BF097732.D
Acq On : 16 Aug 2017 11:04
Operator : SJ/JU
Sample : I4751-10DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-23-COMPDL

Quant Time: Aug 16 12:16:30 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

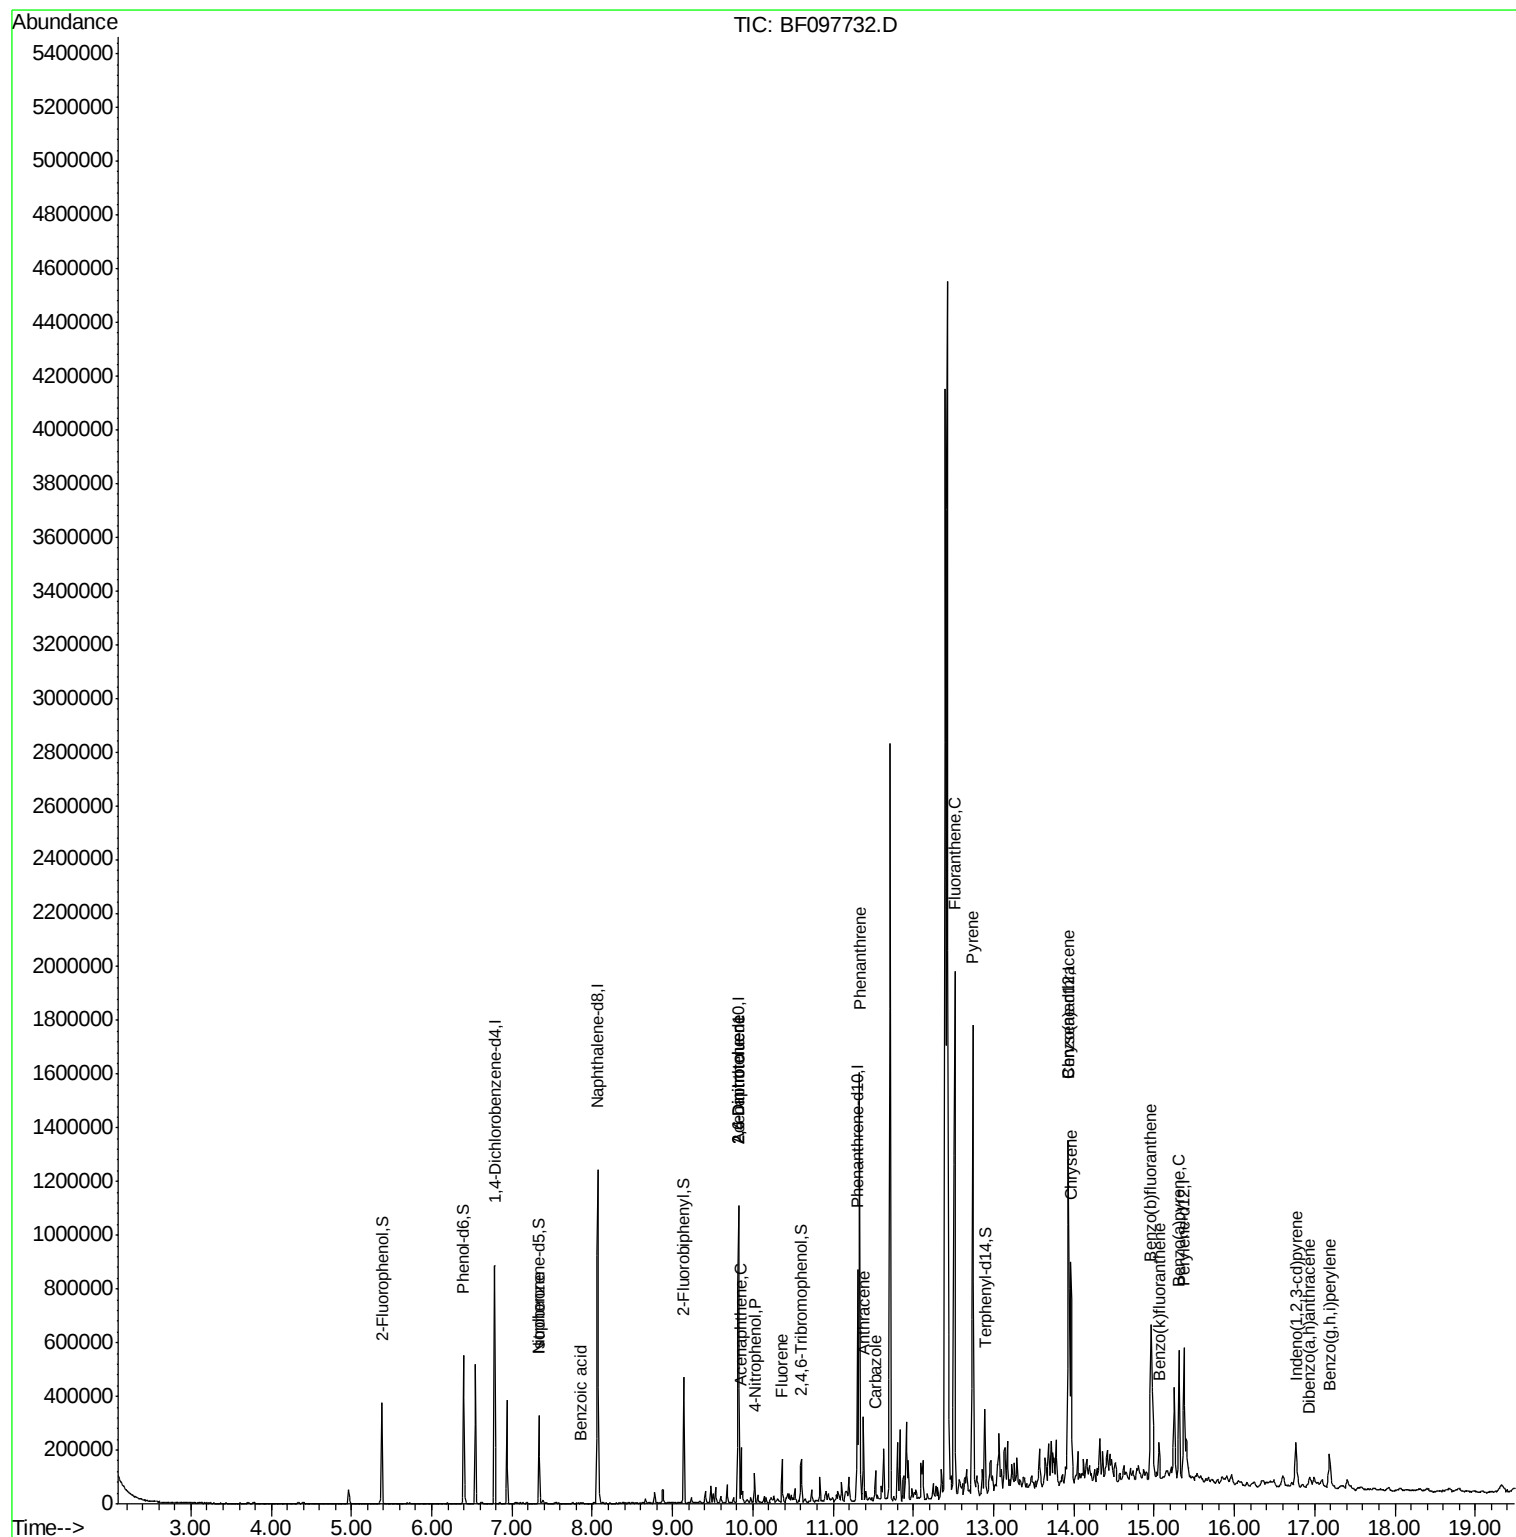







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.79 min Scan# 799
Delta R.T. 0.00 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Instrument :
BNA_F
ClientSampleId :
SB-23-COMPDL




Tgt Ion	Ratio	Lower	Upper
152	100		
150	153.1	126.2	189.2
115	61.7	52.2	78.2

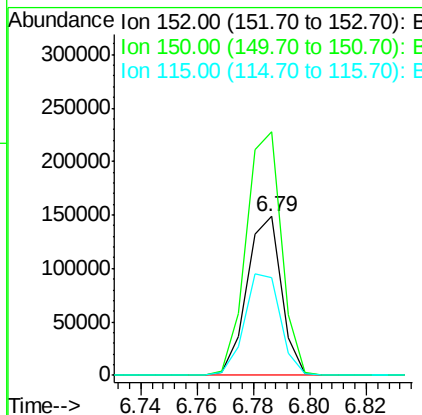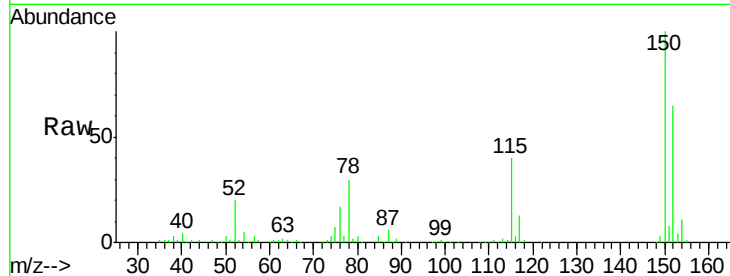


#5

2-Fluorophenol
Concen: 12.130 ng
RT: 5.38 min Scan# 560
Delta R.T. -0.01 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.0	46.0	69.0
63	30.3	23.4	35.0

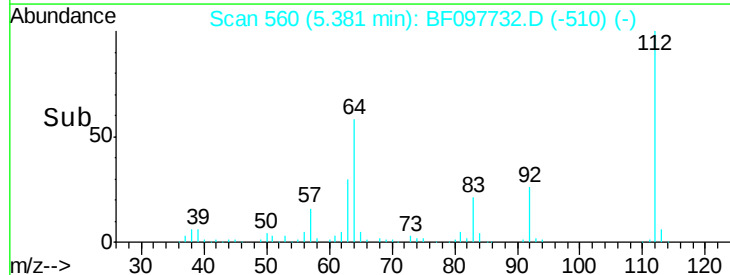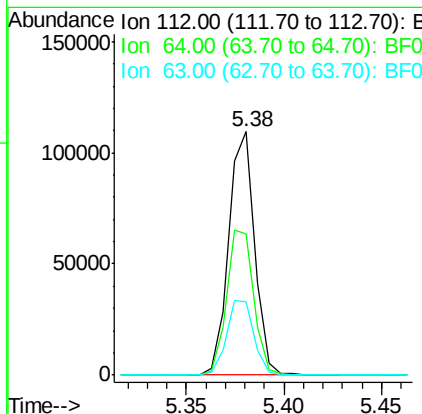

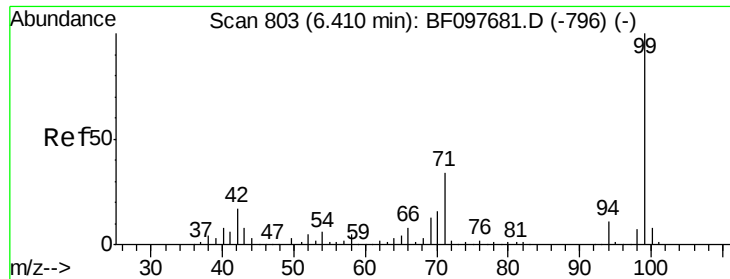

#7

Phenol-d6

Concen: 14.133 ng

RT: 6.40 min Scan# 733

Delta R.T. -0.01 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Instrument :

BNA_F

ClientSampleId :

SB-23-COMPDL


Tgt Ion: 99 Resp: 159008

Ion Ratio Lower Upper

99 100

42 17.9 13.5 20.3




71 35.3 24.5 36.7

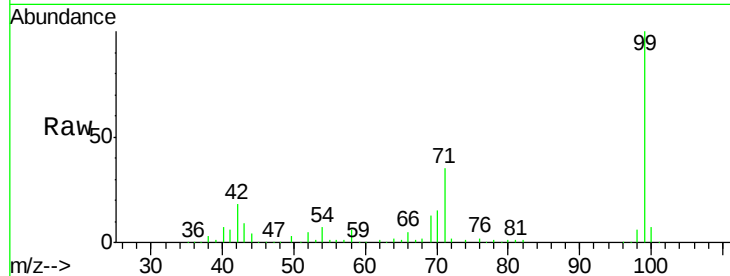

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

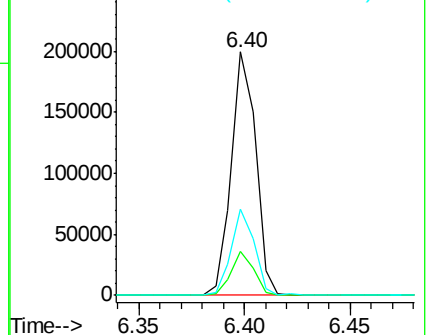

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.07 min Scan# 1017

Delta R.T. 0.00 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Tgt Ion: 136 Resp: 479726


Ion Ratio Lower Upper

136 100

137 11.0 8.5 12.7

54 7.4 4.9 7.3#

68 7.0 4.1 6.1#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

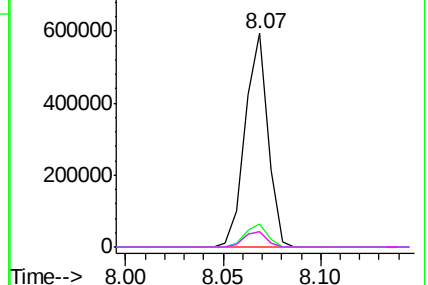







#23
 Nitrobenzene-d5
 Concen: 9.919 ng
 RT: 7.34 min Scan# 893
 Delta R.T. -0.01 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-23-COMPDL

Tgt Ion	Ratio	Lower	Upper
82	100		
128	35.0	34.0	51.0
54	45.6	42.2	63.2

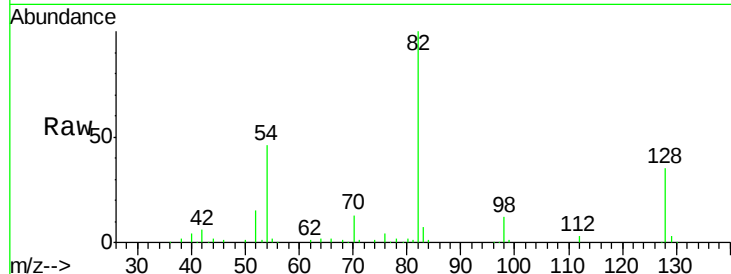


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

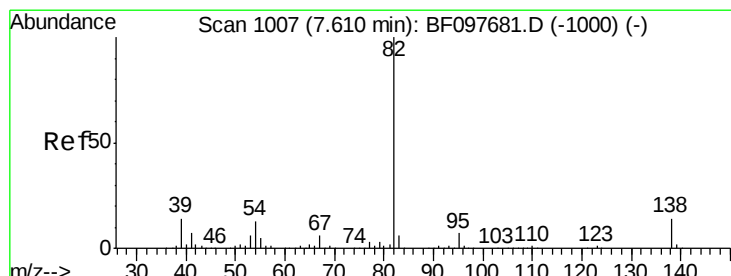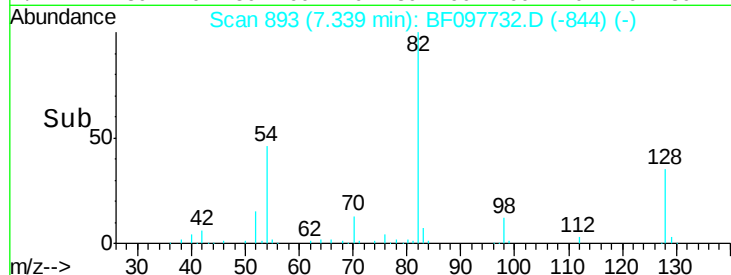
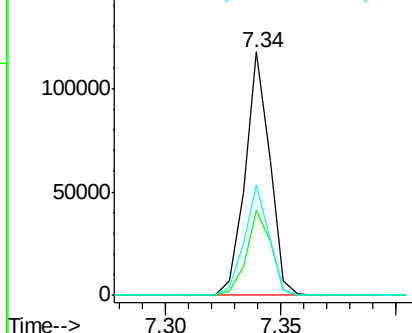



#25
 Isophorone
 Concen: 4.762 ng
 RT: 7.34 min Scan# 893
 Delta R.T. -0.27 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.3	7.9#
138	0.0	13.1	19.7#

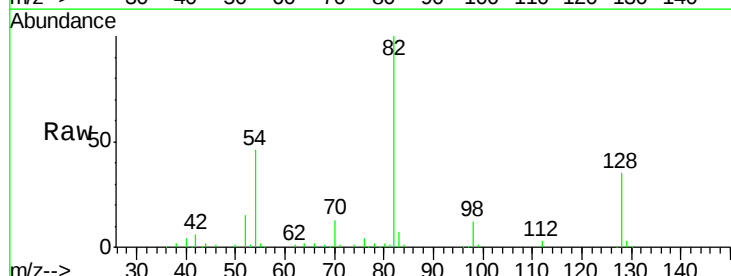

Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 95.00 (94.70 to 95.70): BF0
 Ion 138.00 (137.70 to 138.70): BF0

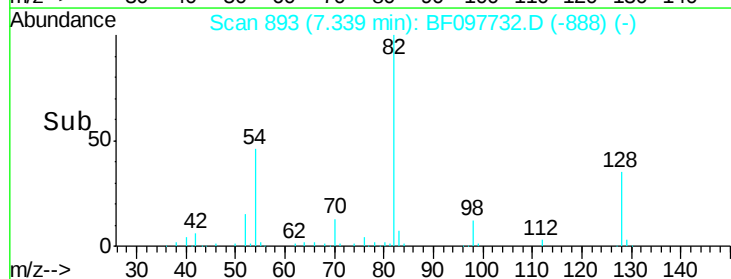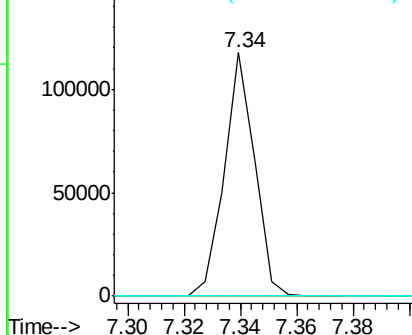

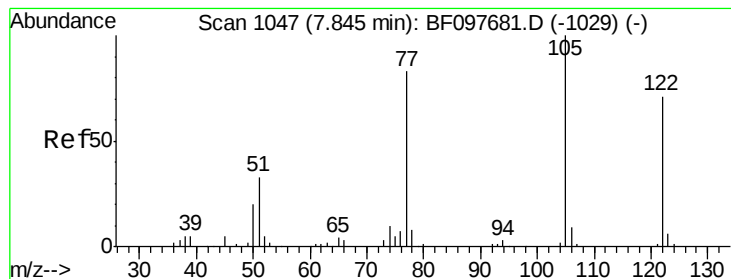

#32

Benzoic acid

Concen: 6.427 ng

RT: 7.85 min Scan# 980

Delta R.T. 0.01 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Instrument :


BNA_F

ClientSampleId :

SB-23-COMPDL

Tgt Ion:122 Resp: 144




Ion	Ratio	Lower	Upper
122	100		
105	0.0	103.3	143.3#
77	0.0	73.7	113.7#



Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF0

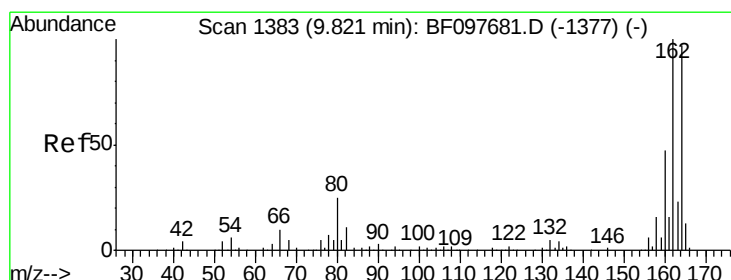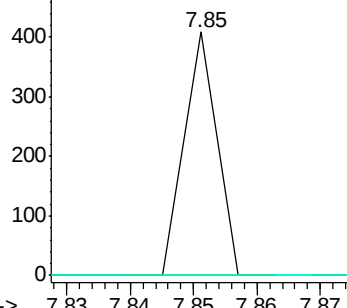

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.82 min Scan# 1315


Delta R.T. 0.00 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Tgt Ion:164 Resp: 187131



Ion	Ratio	Lower	Upper
164	100		
162	103.5	82.6	123.8
160	47.5	36.2	54.2

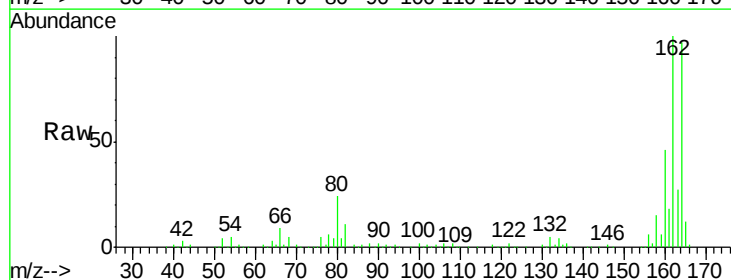


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E




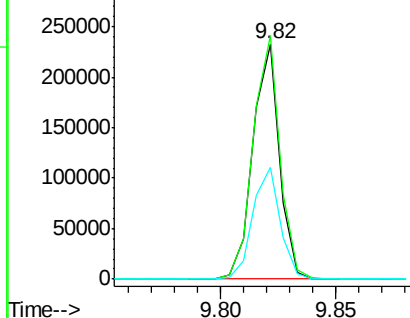


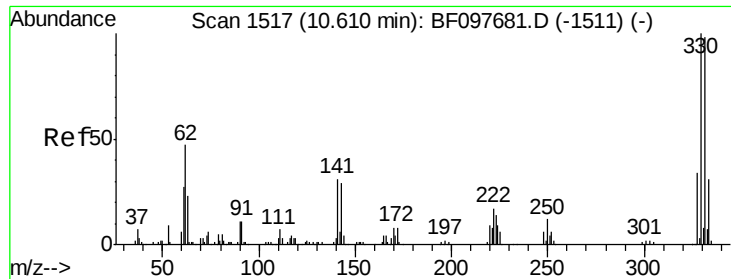

#41
 2,4,6-Tribromophenol
 Concen: 5.918 ng
 RT: 10.60 min Scan# 1448
 Delta R.T. -0.01 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04




Instrument :
 BNA_F
 ClientSampleId :
 SB-23-COMPDL


Tgt Ion: 330 Resp: 9609
 Ion Ratio Lower Upper
 330 100
 332 100.2 76.6 115.0
 141 51.7 31.4 47.2#

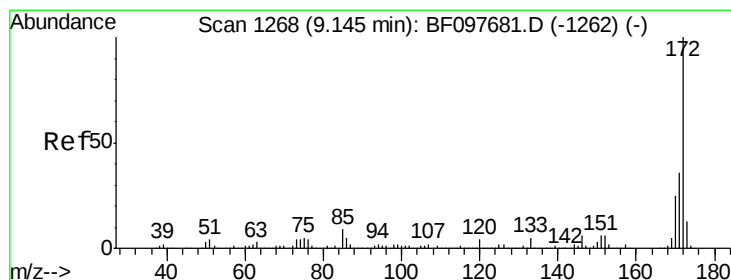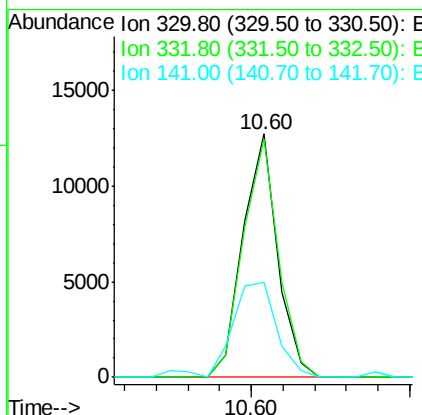

#44
 2-Fluorobiphenyl
 Concen: 9.913 ng
 RT: 9.14 min Scan# 1199
 Delta R.T. -0.01 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Tgt Ion: 172 Resp: 126266
 Ion Ratio Lower Upper
 172 100
 171 34.8 29.6 44.4
 170 23.1 19.8 29.8

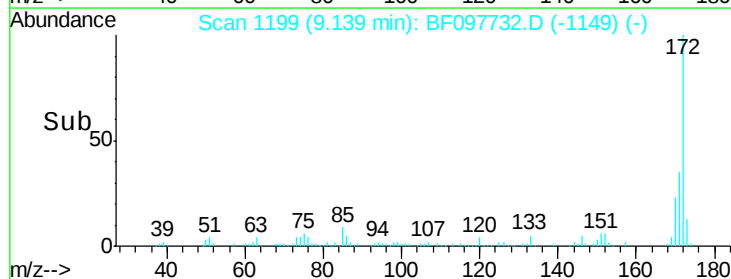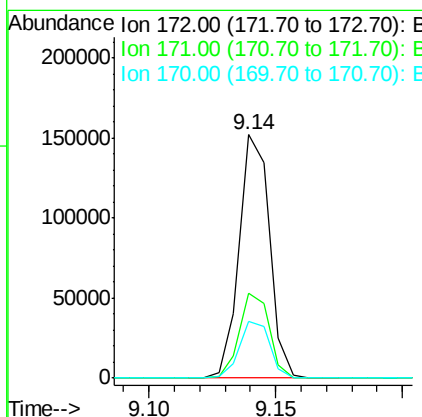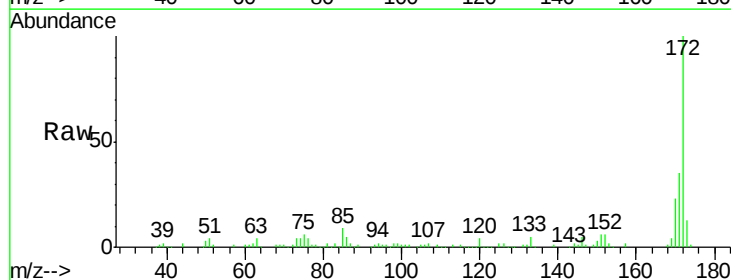







#50
 2,6-Dinitrotoluene
 Concen: 8.932 ng
 RT: 9.82 min Scan# 1315
 Delta R.T. 0.21 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Instrument :
 BNA_F
 ClientSampleId :
 SB-23-COMPDL

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	34.3	51.5#
89	2.2	37.1	55.7#

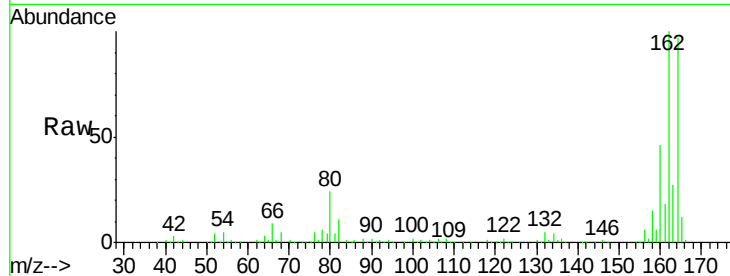


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

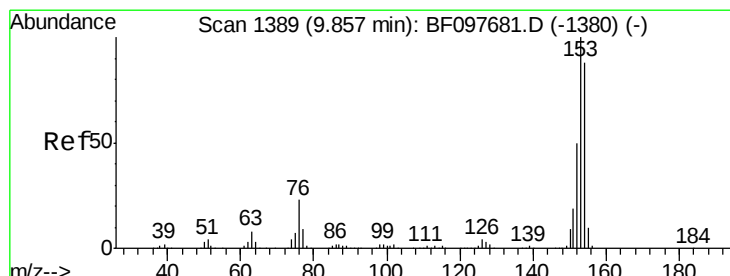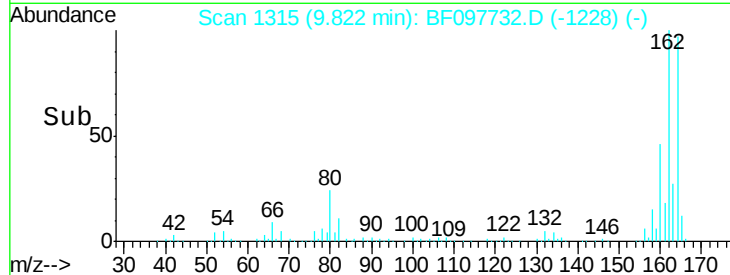
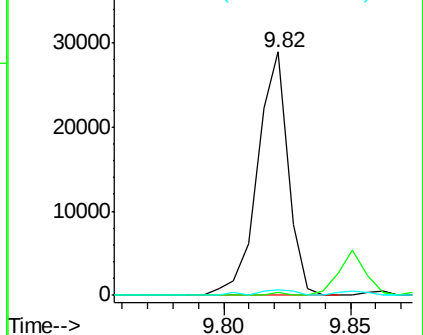



#51
 Acenaphthene
 Concen: 2.867 ng
 RT: 9.85 min Scan# 1320
 Delta R.T. -0.01 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Tgt Ion	Ratio	Lower	Upper
154	100		
153	116.3	90.5	135.7
152	53.7	43.6	65.4

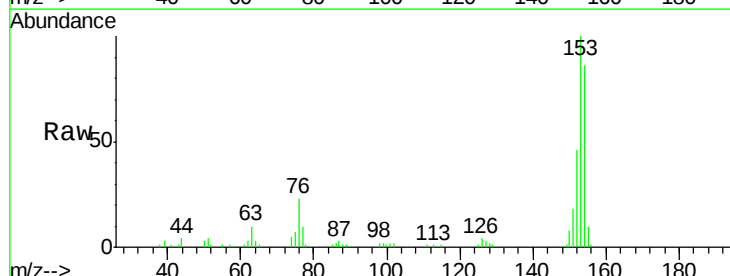

Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 152.00 (151.70 to 152.70): E

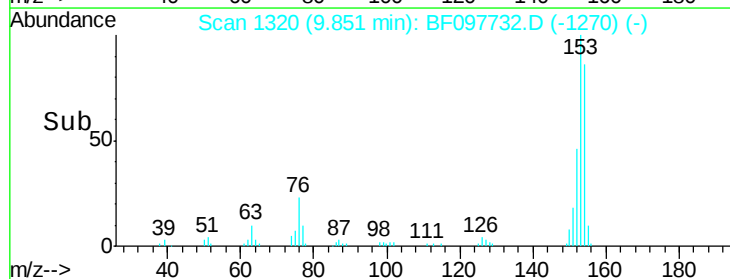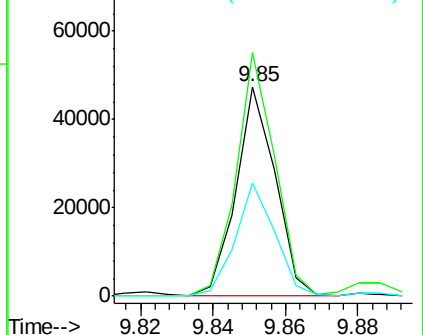


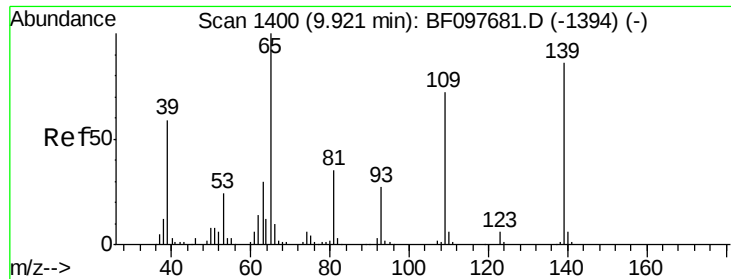




#55
4-Nitrophenol
Concen: 3.589 ng
RT: 10.02 min Scan# 1349
Delta R.T. 0.10 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Instrument :
BNA_F
ClientSampleId :
SB-23-COMPDL

Tgt Ion	Ratio	Lower	Upper
139	100		
109	0.0	34.1	74.1#
65	3.2	31.4	71.4#




Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF0


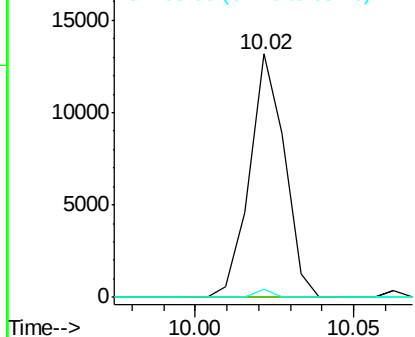



#56
2,4-Dinitrotoluene
Concen: 7.117 ng
RT: 9.82 min Scan# 1315
Delta R.T. -0.18 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	25.4	38.0#
89	2.2	46.4	69.6#
182	0.0	1.8	2.6#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0
Ion 182.00 (181.70 to 182.70): E




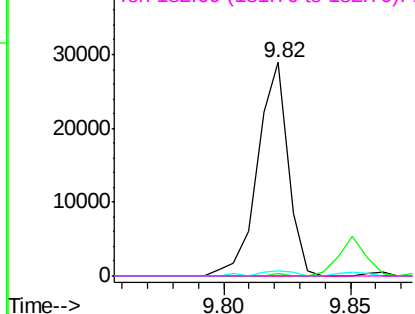


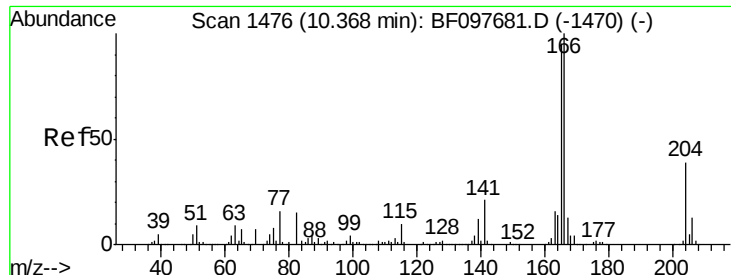

#57
 Fluorene
 Concen: 2.895 ng
 RT: 10.36 min Scan# 1407
 Delta R.T. -0.01 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04




Instrument :
 BNA_F
 ClientSampleId :
 SB-23-COMPDL


Tgt Ion:166 Resp: 37457
 Ion Ratio Lower Upper
 166 100
 165 99.7 78.8 118.2
 167 15.4 10.6 16.0

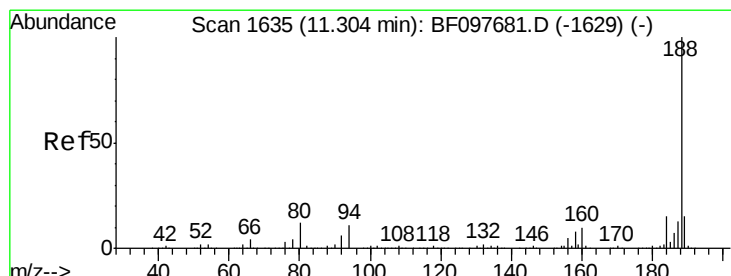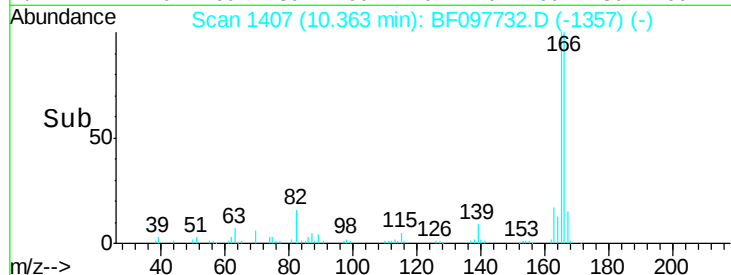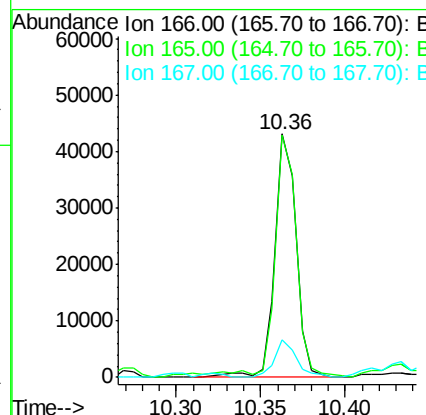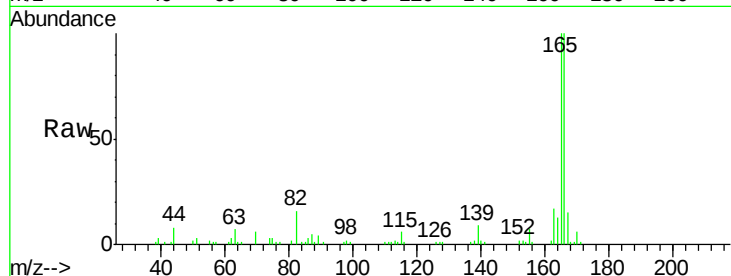

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.30 min Scan# 1567
 Delta R.T. 0.00 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Tgt Ion:188 Resp: 277710
 Ion Ratio Lower Upper
 188 100
 94 11.6 9.4 14.2
 80 12.7 10.2 15.2

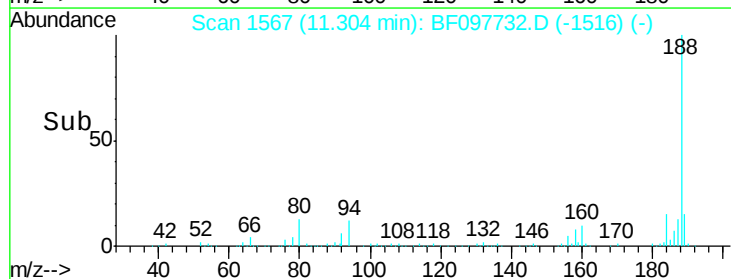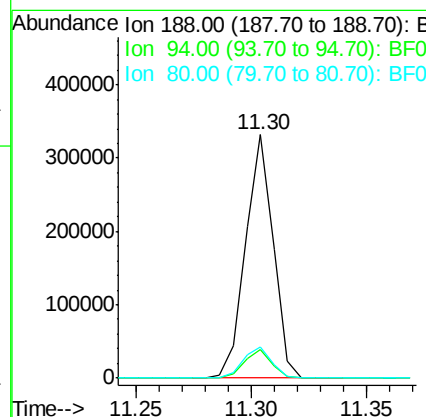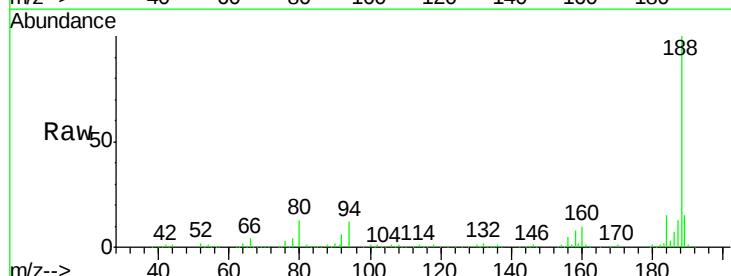


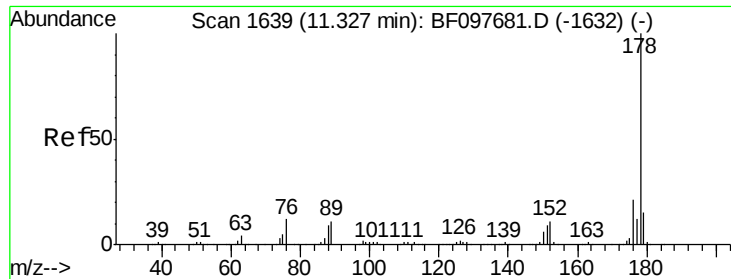




#70
Phenanthrene
Concen: 33.853 ng
RT: 11.33 min Scan# 1571
Delta R.T. 0.00 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Instrument :
BNA_F
ClientSampleId :
SB-23-COMPDL

Tgt Ion:178 Resp: 500968
Ion Ratio Lower Upper
178 100
176 19.9 16.2 24.4
179 15.7 12.6 19.0

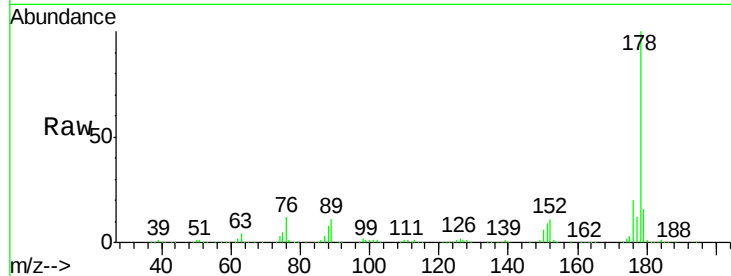


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E


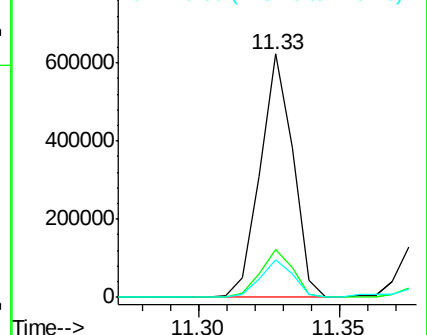



#71
Anthracene
Concen: 7.308 ng
RT: 11.37 min Scan# 1579
Delta R.T. -0.01 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Tgt Ion:178 Resp: 109689
Ion Ratio Lower Upper
178 100
176 18.5 15.8 23.8
179 15.1 12.7 19.1



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

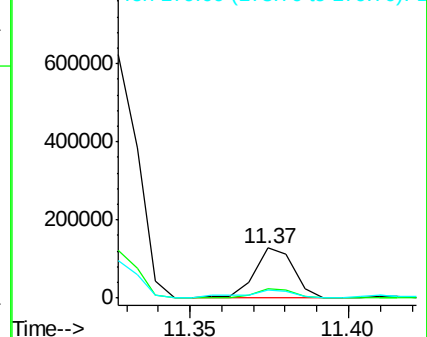



#72

Carbazole

Concen: 2.740 ng

RT: 11.53 min Scan# 1605

Delta R.T. -0.01 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Instrument :

BNA_F

ClientSampleId :

SB-23-COMPDL


Tgt Ion:167 Resp: 39035

Ion Ratio Lower Upper

167 100

166 22.4 18.1 27.1




139 14.1 11.7 17.5



Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

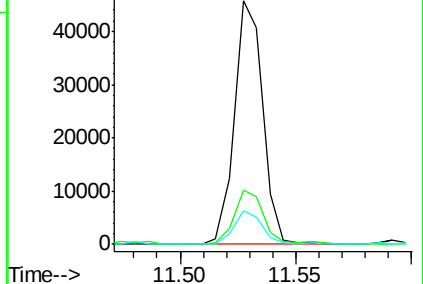

#74

Fluoranthene

Concen: 44.467 ng

RT: 12.52 min Scan# 1773

Delta R.T. 0.01 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04


Tgt Ion:202 Resp: 686845

Ion Ratio Lower Upper

202 100

101 14.3 0.0 33.2



203 18.0 0.0 38.1




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

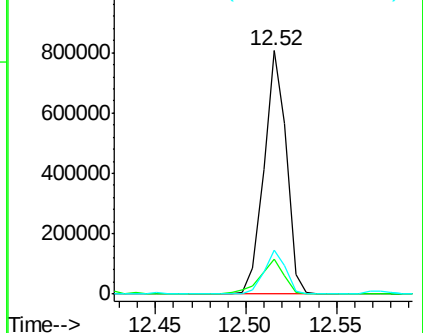



#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.94 min Scan# 2015

Delta R.T. 0.00 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Instrument :

BNA_F

ClientSampleId :

SB-23-COMPDL


Tgt Ion:240 Resp: 264079

Ion Ratio Lower Upper

240 100

120 14.2 5.8 8.8#




236 26.8 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

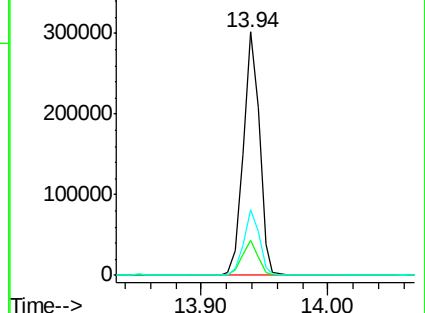

#77

Pyrene

Concen: 30.174 ng

RT: 12.74 min Scan# 1812

Delta R.T. 0.01 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04


Tgt Ion:202 Resp: 651727

Ion Ratio Lower Upper

202 100

200 20.6 17.6 26.4



203 17.7 14.4 21.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E



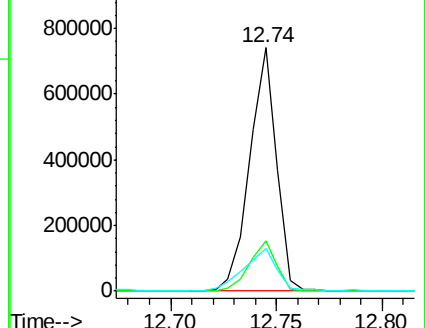





#78
 Terphenyl-d14
 Concen: 5.933 ng
 RT: 12.89 min Scan# 1836
 Delta R.T. -0.01 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04




Instrument :
 BNA_F
 ClientSampleId :
 SB-23-COMPDL


Tgt Ion: 244 Resp: 75137
 Ion Ratio Lower Upper
 244 100
 212 8.4 6.0 9.0
 122 14.5 10.3 15.5

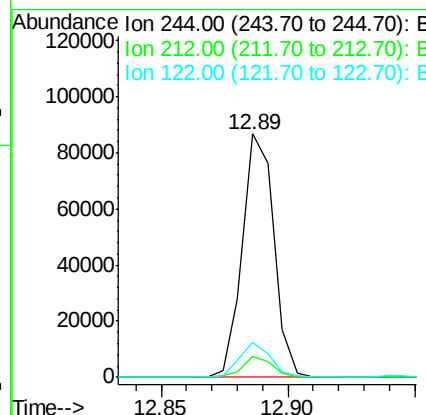

#80
 Benzo(a)anthracene
 Concen: 21.286 ng
 RT: 13.93 min Scan# 2013
 Delta R.T. 0.00 min
 Lab File: BF097732.D
 Acq: 16 Aug 2017 11:04

Tgt Ion: 228 Resp: 336894
 Ion Ratio Lower Upper
 228 100
 226 30.8 22.6 33.8
 229 21.2 16.3 24.5

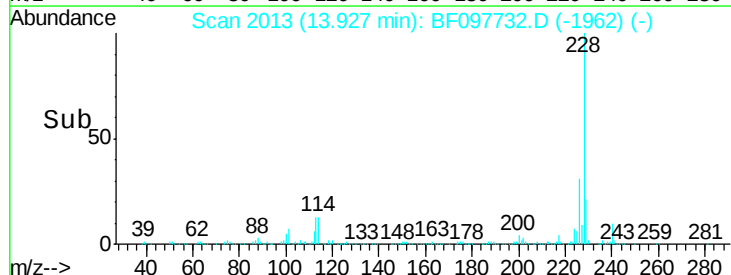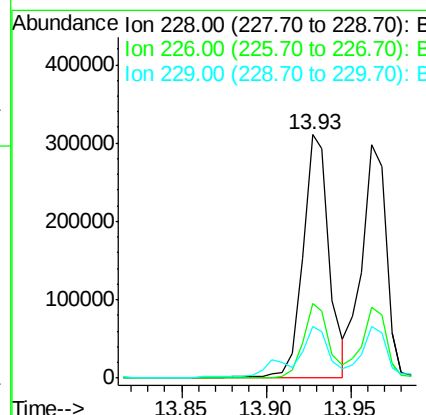



#82

Chrysene

Concen: 19.084 ng

RT: 13.96 min Scan# 2019

Delta R.T. 0.00 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Instrument :

BNA_F

ClientSampleId :

SB-23-COMPDL


Tgt Ion:228 Resp: 300465

Ion Ratio Lower Upper

228 100

226 30.3 24.9 37.3




229 22.0 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

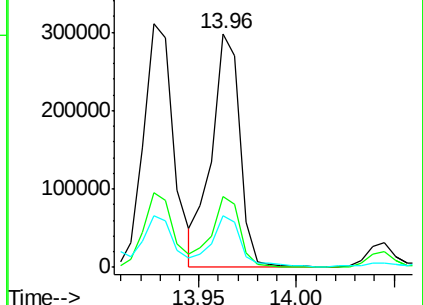

#85

Indeno(1,2,3-cd)pyrene

Concen: 8.847 ng

RT: 16.77 min Scan# 2496

Delta R.T. 0.01 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04


Tgt Ion:276 Resp: 102465

Ion Ratio Lower Upper

276 100

138 25.1 27.8 41.6#



277 24.3 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



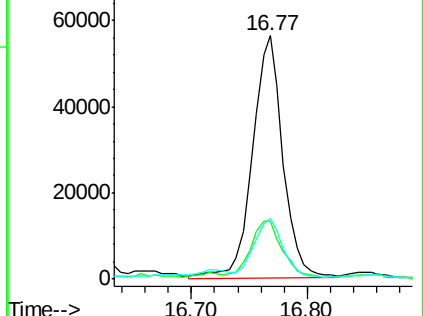



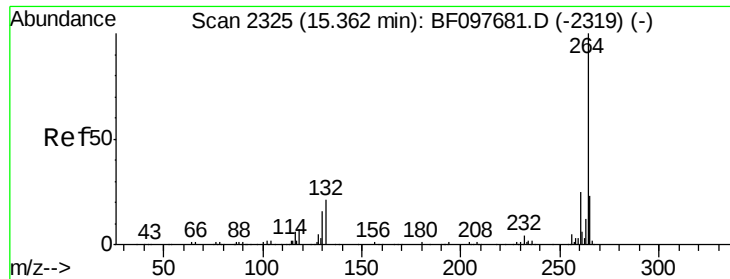

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.37 min Scan# 2259
Delta R.T. 0.01 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04




Instrument :
BNA_F
ClientSampleId :
SB-23-COMPDL


Tgt Ion:264 Resp: 206614
Ion Ratio Lower Upper
264 100
260 23.8 19.5 29.3
265 22.1 17.2 25.8

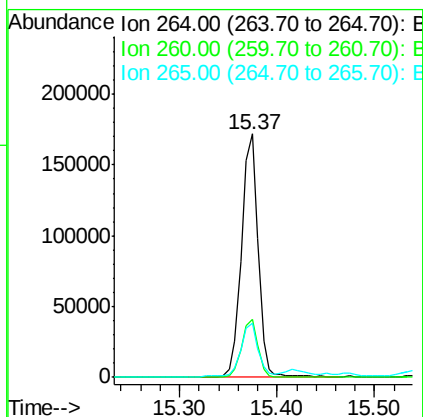

#87
Benzo(b)fluoranthene
Concen: 32.794 ng
RT: 14.96 min Scan# 2189
Delta R.T. 0.01 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Tgt Ion:252 Resp: 427100
Ion Ratio Lower Upper
252 100
253 23.0 18.1 27.1
125 11.8 9.8 14.8



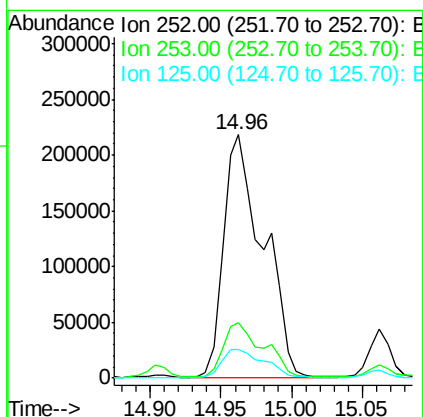



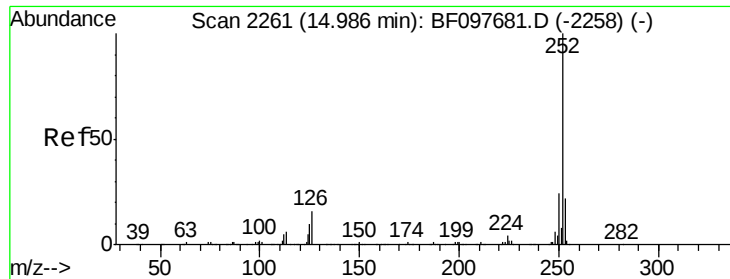

#88
Benzo(k)fluoranthene
Concen: 3.780 ng
RT: 15.06 min Scan# 2206
Delta R.T. 0.08 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04




Instrument :
BNA_F
ClientSampleId :
SB-23-COMPDL


Tgt Ion:252 Resp: 46246
Ion Ratio Lower Upper
252 100
253 26.0 18.4 27.6
125 16.1 13.1 19.7

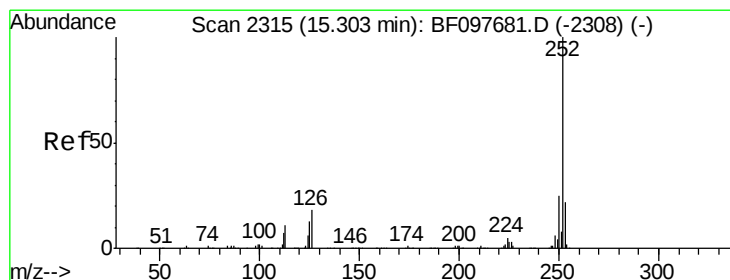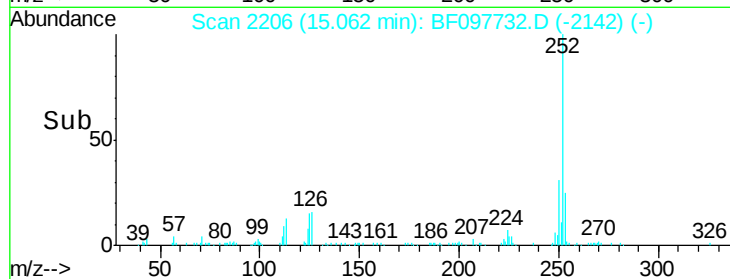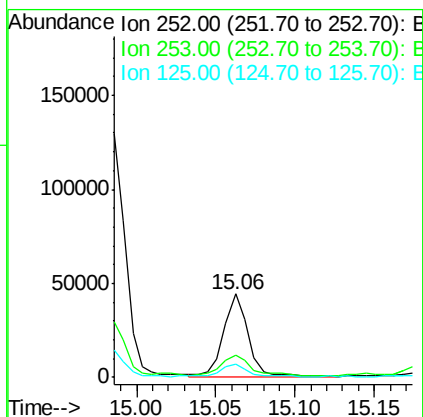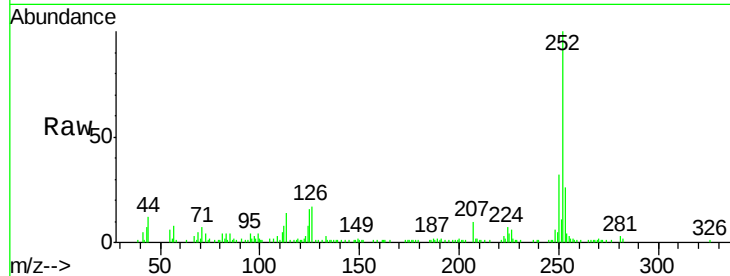

#89
Benzo(a)pyrene
Concen: 18.945 ng
RT: 15.31 min Scan# 2248
Delta R.T. 0.01 min
Lab File: BF097732.D
Acq: 16 Aug 2017 11:04

Tgt Ion:252 Resp: 218429
Ion Ratio Lower Upper
252 100
253 23.1 17.5 26.3
125 12.3 11.0 16.4

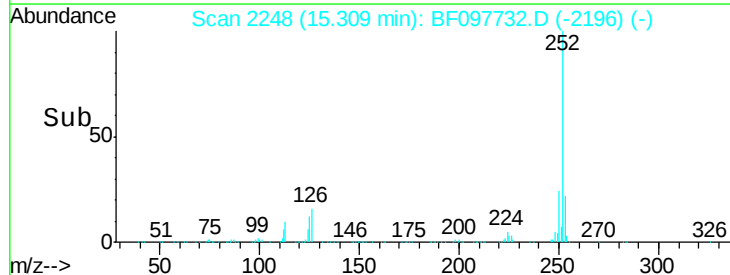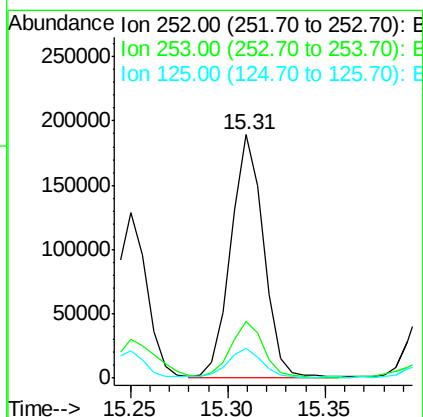

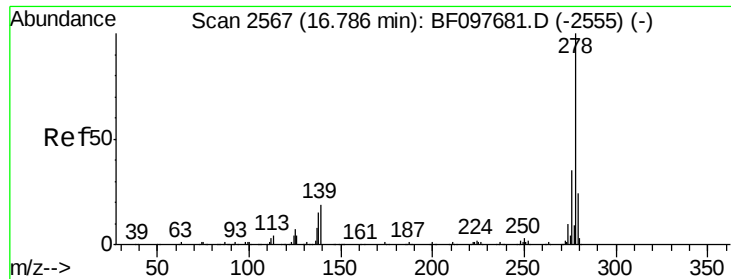

#90

Dibenzo(a,h)anthracene

Concen: 2.137 ng

RT: 16.94 min Scan# 2525

Delta R.T. 0.15 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04

Instrument :

BNA_F

ClientSampleId :

SB-23-COMPDL


Tgt Ion: 278 Resp: 20059

Ion Ratio Lower Upper

278 100

139 24.3 16.6 24.8




279 26.4 19.3 28.9

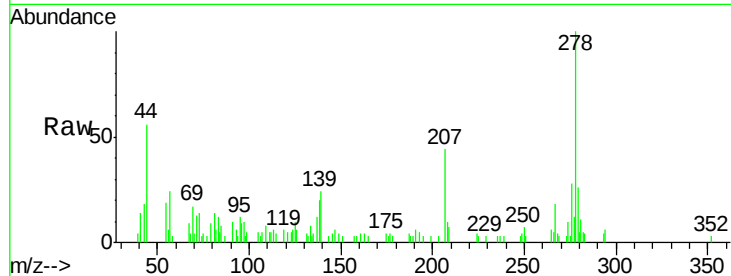

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

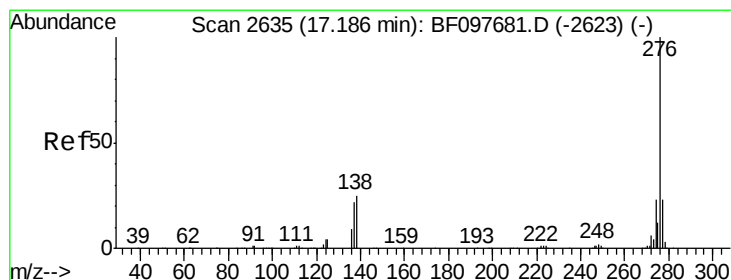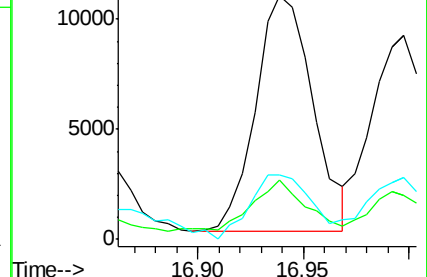

#91

Benzo(g,h,i)perylene

Concen: 9.567 ng

RT: 17.19 min Scan# 2567

Delta R.T. 0.00 min

Lab File: BF097732.D

Acq: 16 Aug 2017 11:04


Tgt Ion: 276 Resp: 93694

Ion Ratio Lower Upper

276 100

277 22.7 18.6 28.0

138 25.8 25.4 38.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

