



Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081517.M  
Calibration Table Last Updated: Tue Aug 15 13:25:08 2017

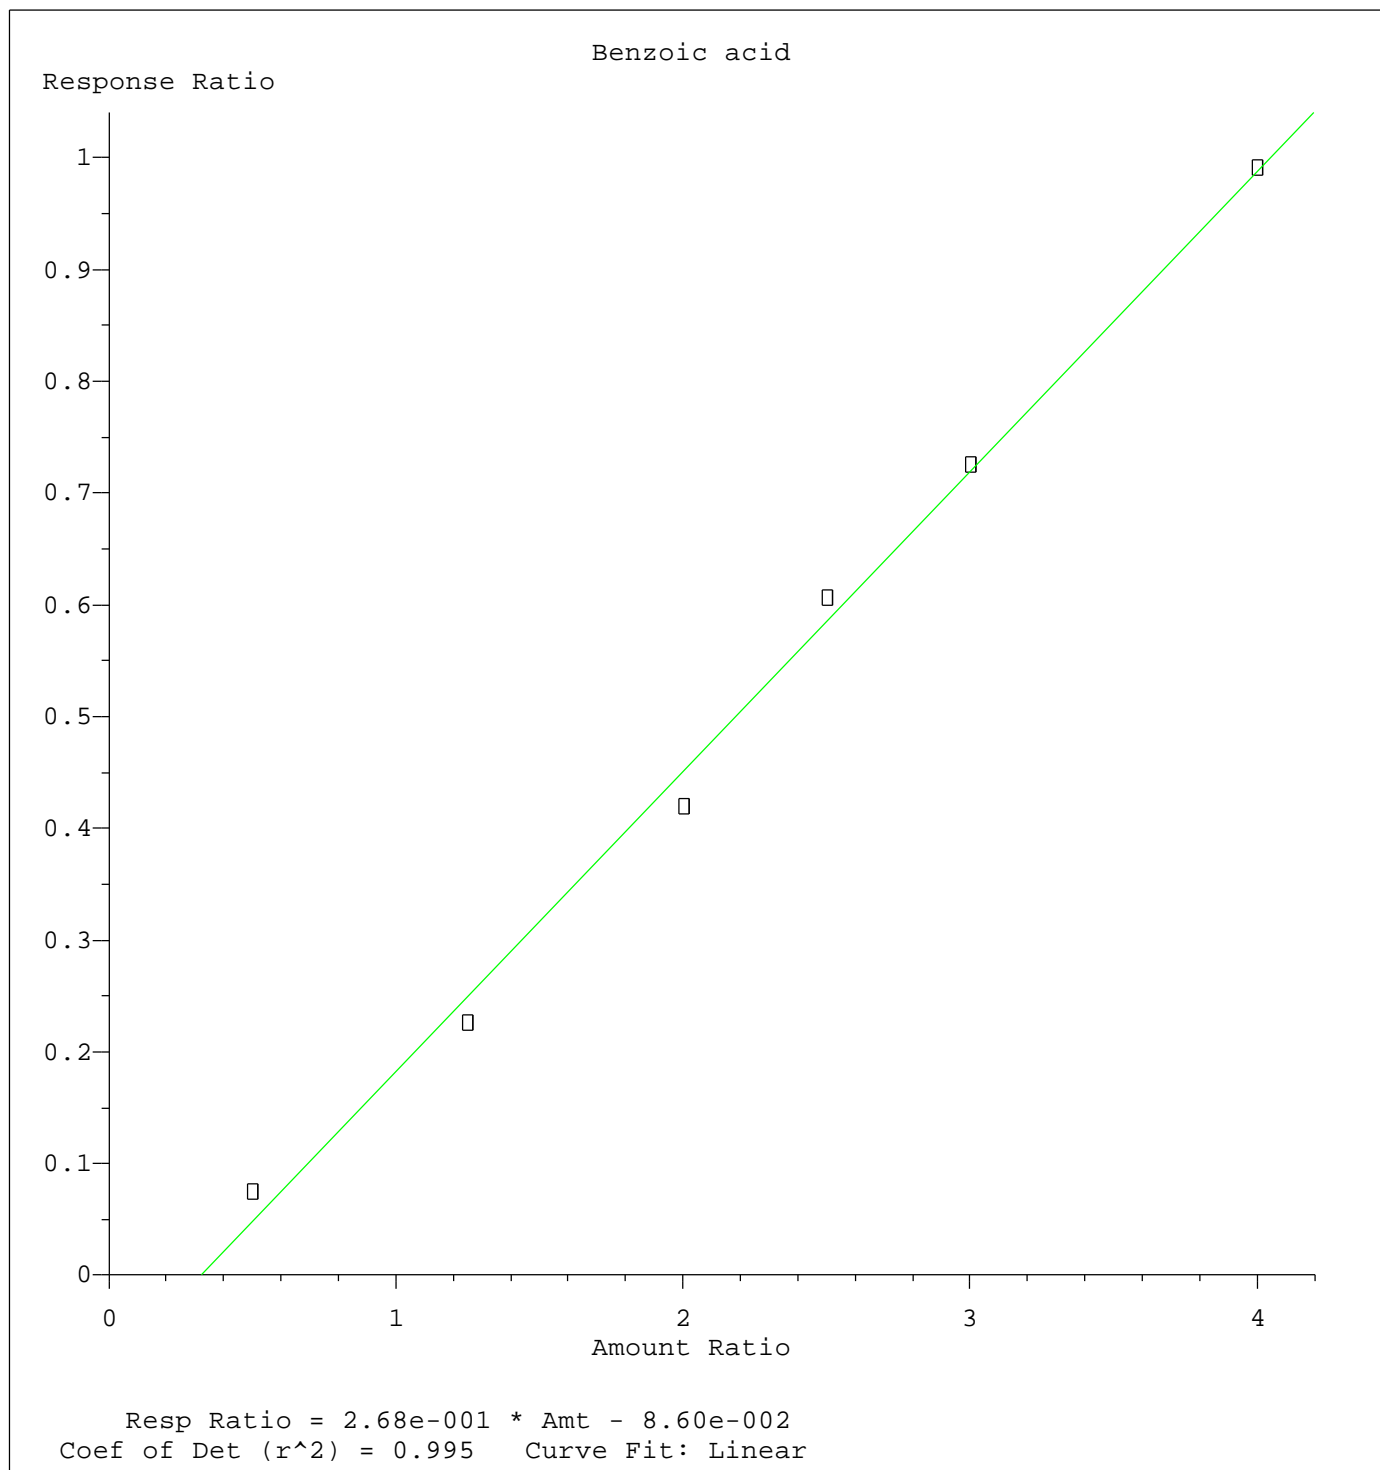

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081517.M  
Calibration Table Last Updated: Tue Aug 15 13:25:08 2017


2,4-Dinitrophenol

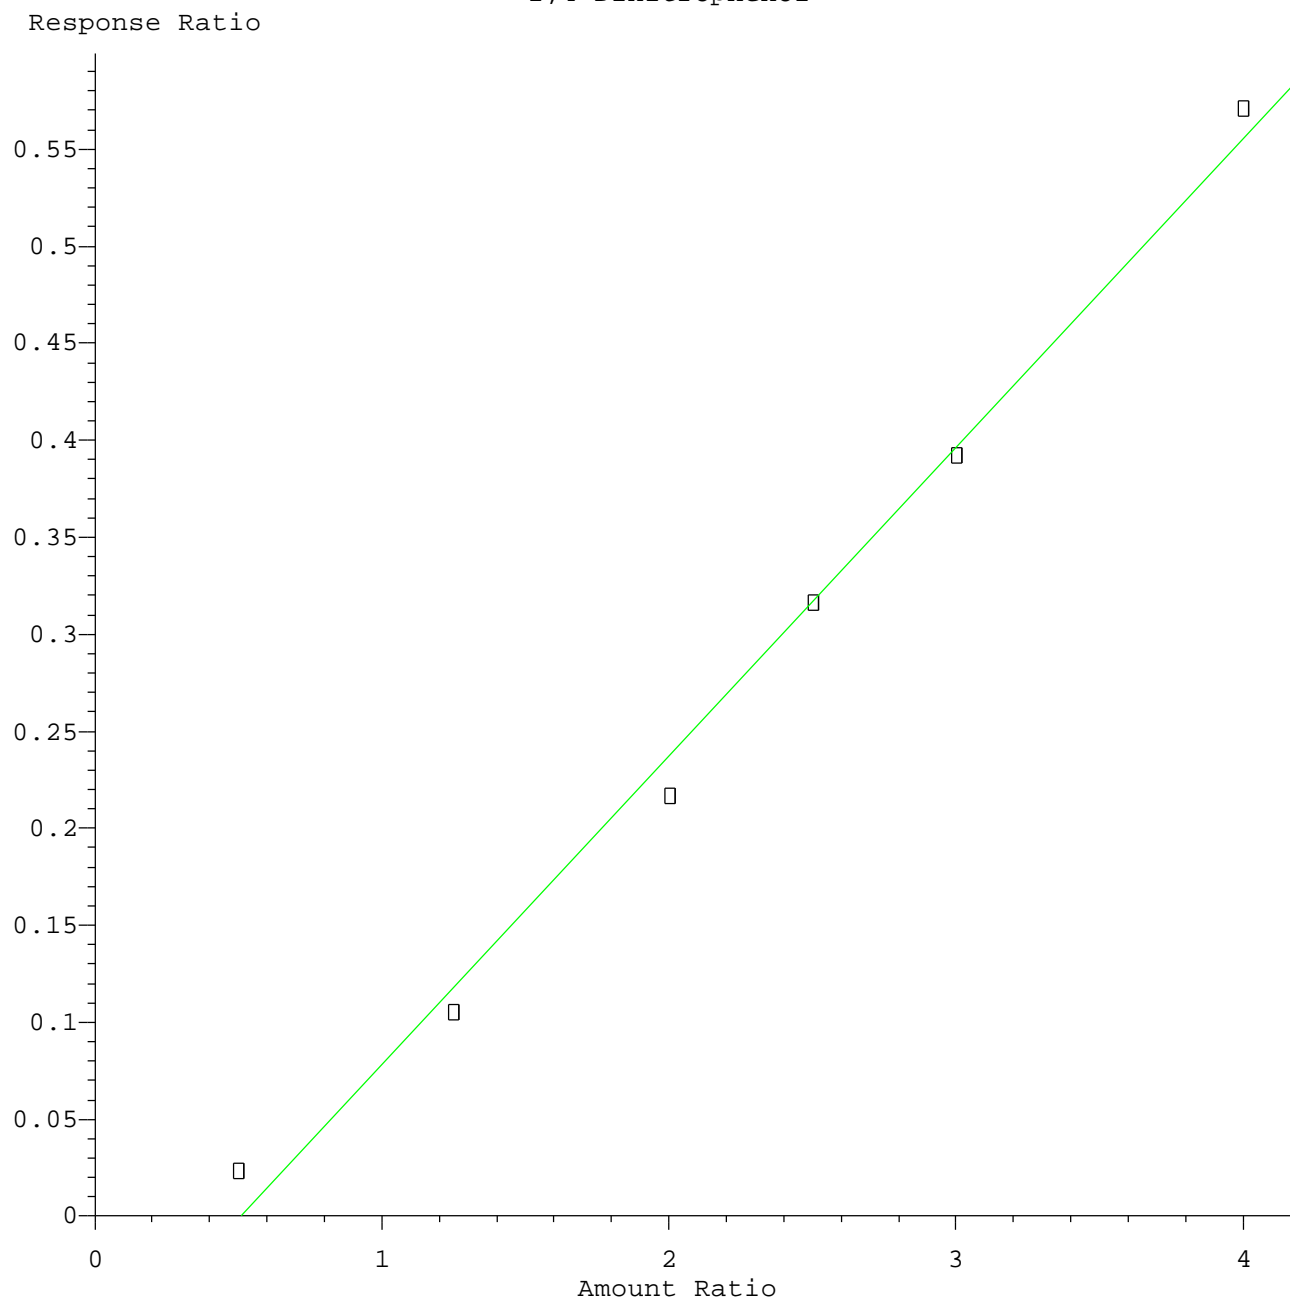

Resp Ratio =  $1.59 \times 10^{-1} \times \text{Amt} - 8.06 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.993    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081517.M  
Calibration Table Last Updated: Tue Aug 15 13:25:08 2017

4,6-Dinitro-2-methylphenol

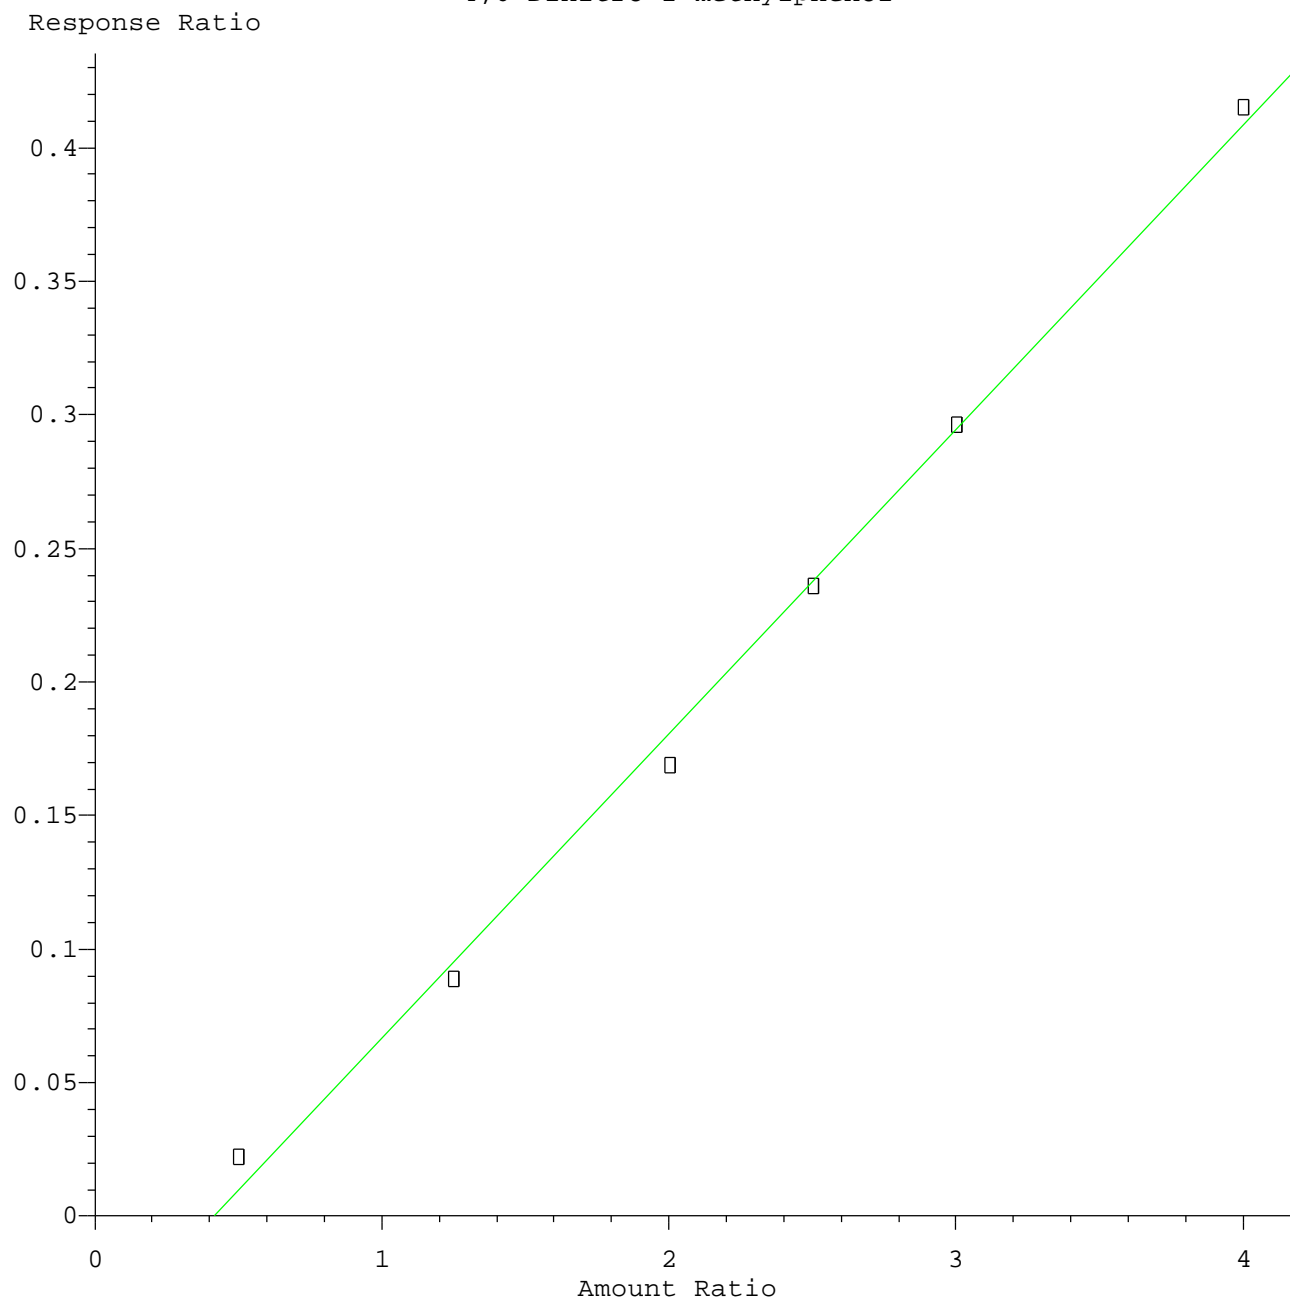

Resp Ratio =  $1.14 \times 10^{-1} \times \text{Amt} - 4.74 \times 10^{-2}$   
Coef of Det ( $r^2$ ) = 0.996    Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081517.M  
Calibration Table Last Updated: Tue Aug 15 13:25:08 2017