
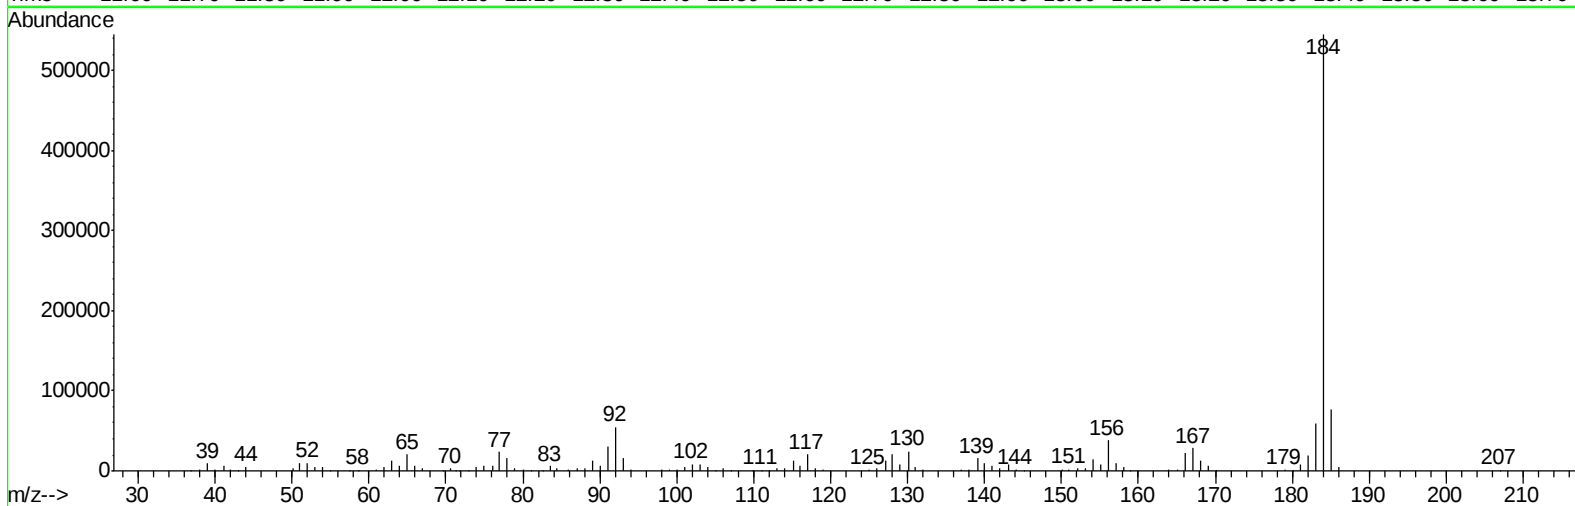


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081517\
Data File : BF097677.D
Acq On : 15 Aug 2017 8:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 07:10:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

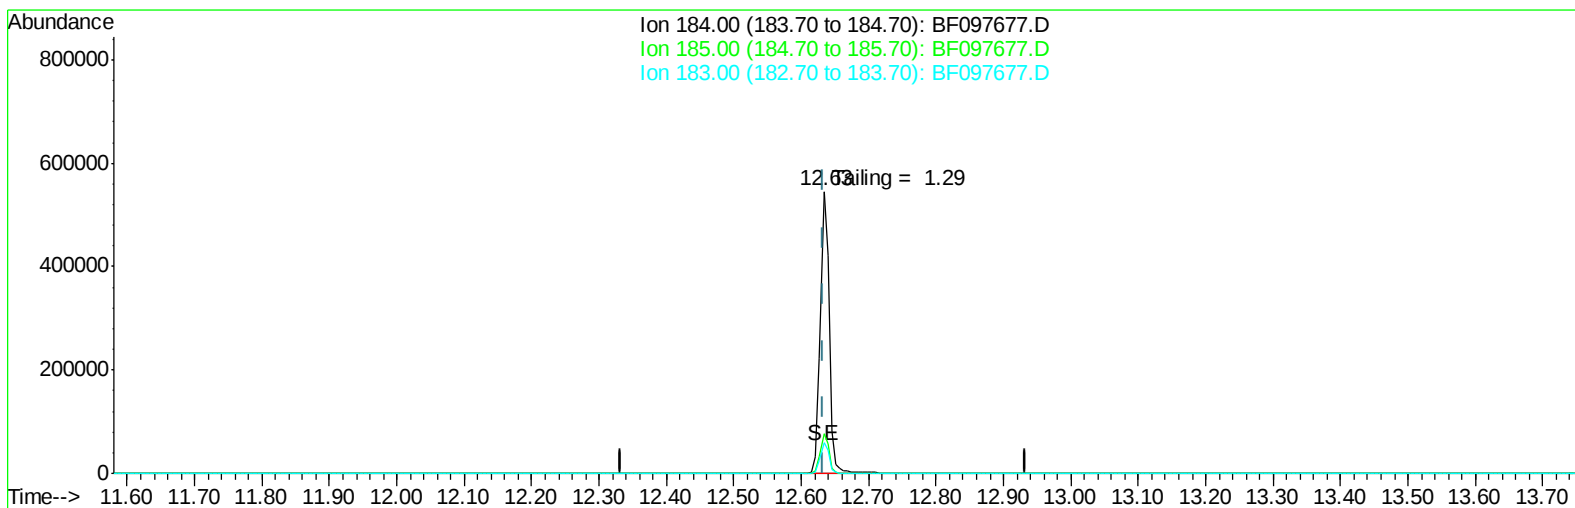

TIC: BF097677.D

(76) Benzidine



12.633min (-0.000) 0.00ng

response 480526

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.02#
183.00	12.20	10.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081517\
Data File : BF097677.D
Acq On : 15 Aug 2017 8:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 07:10:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

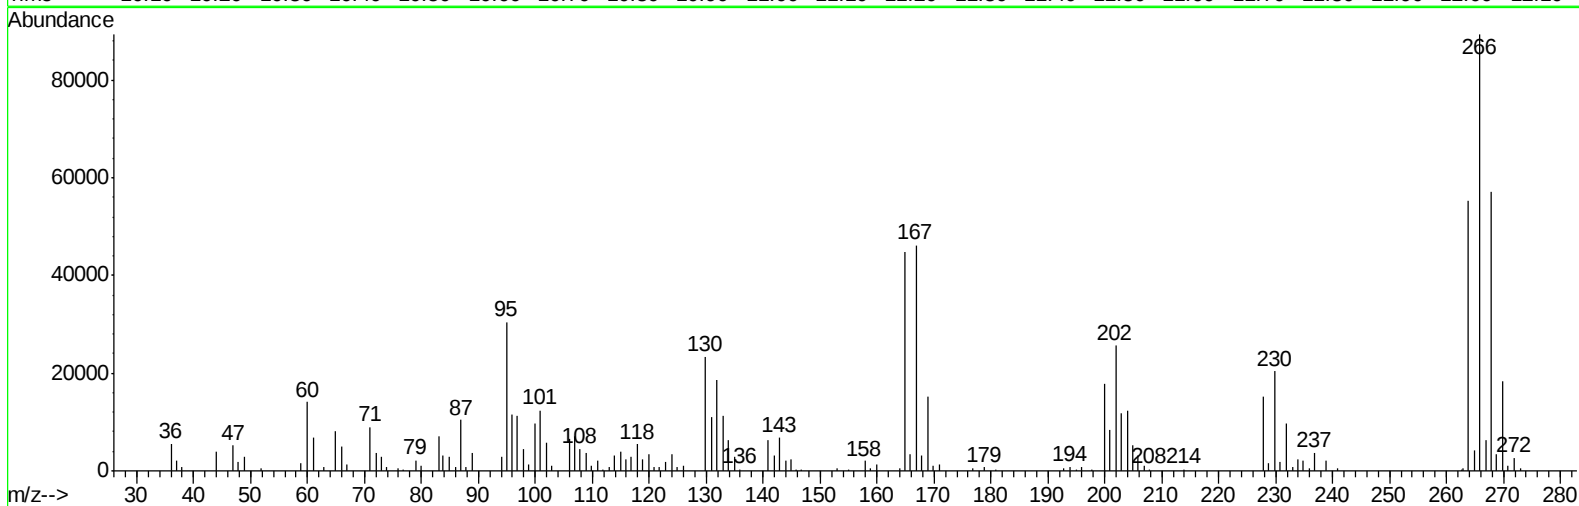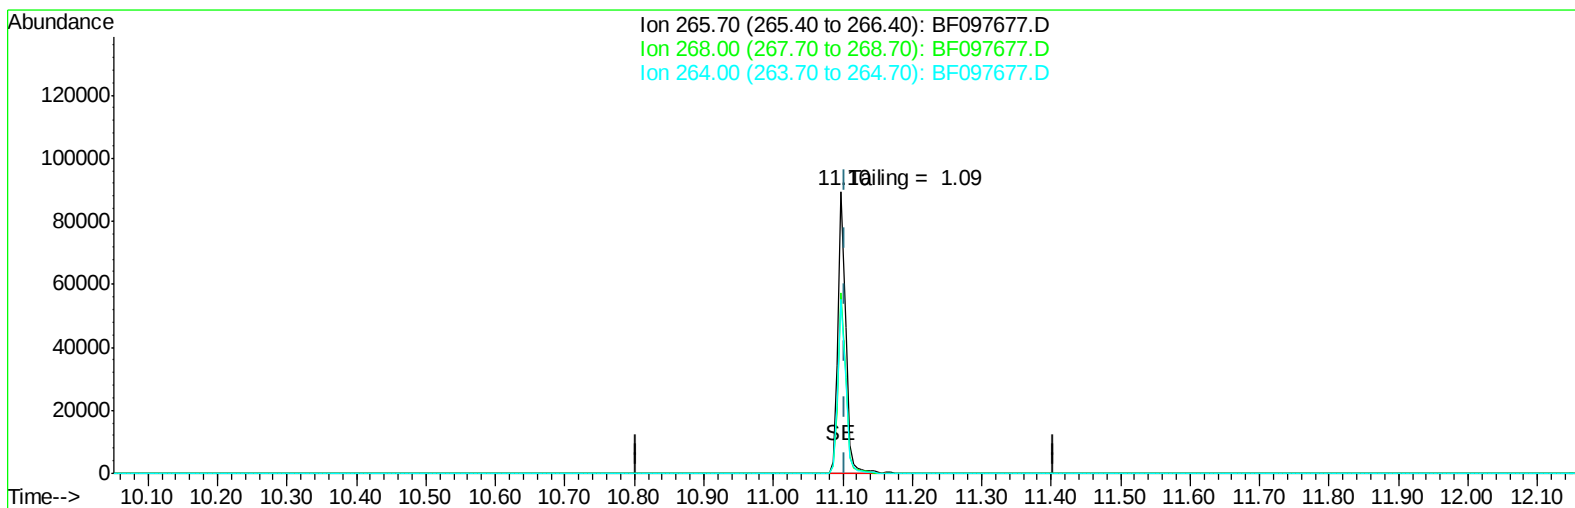

TIC: BF097677.D

(69) Pentachlorophenol (C)

11.098min (-0.006) 41555.91ng

response 67191

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.04
264.00	64.60	61.94
0.00	0.00	0.00