
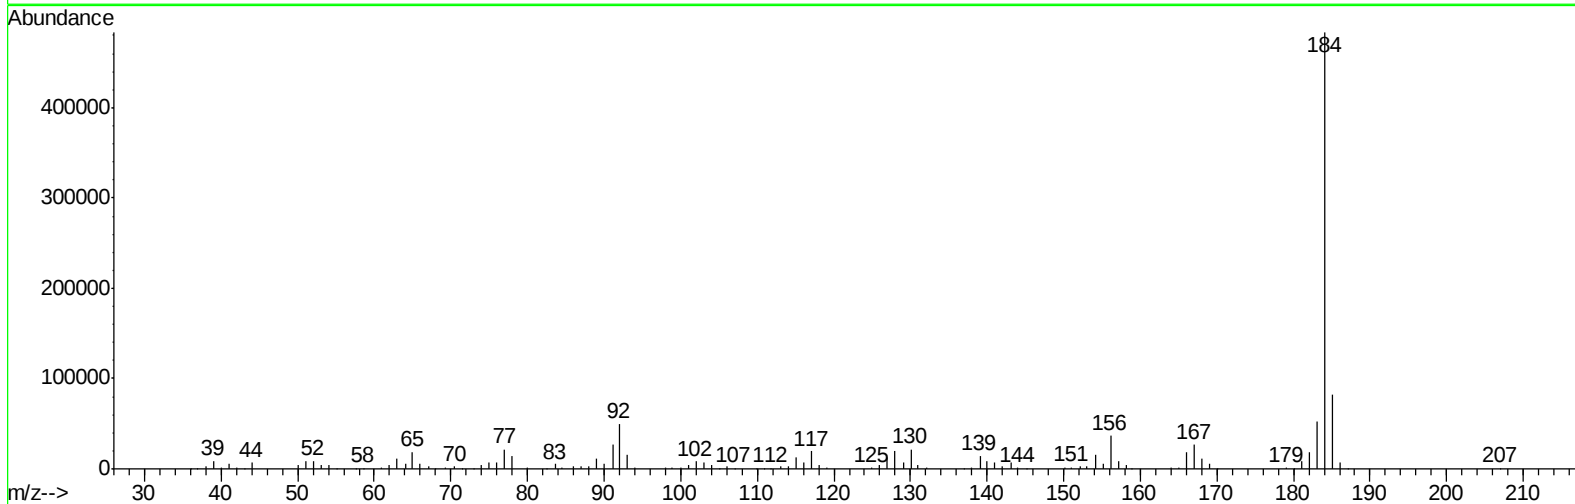


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081517\
Data File : BF097686.D
Acq On : 15 Aug 2017 12:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 07:24:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

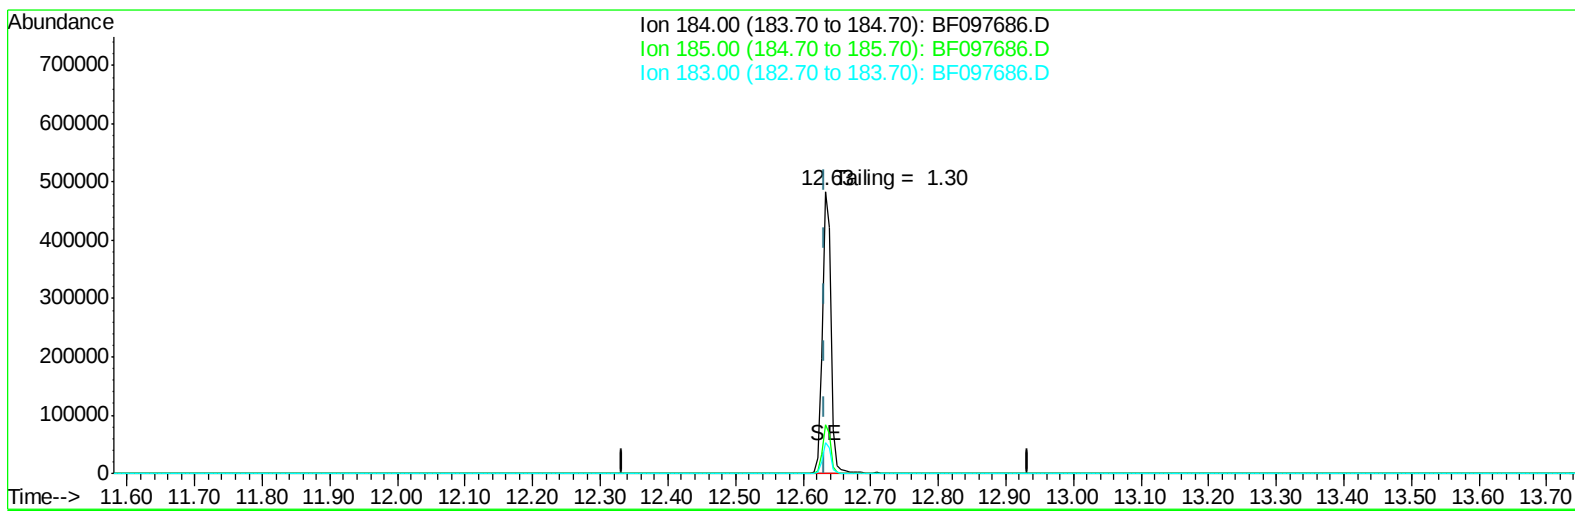

TIC: BF097686.D

(76) Benzidine



12.633min (+0.000) 48254.55ng

response 439840

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	17.06
183.00	12.20	10.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081517\
Data File : BF097686.D
Acq On : 15 Aug 2017 12:57
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 07:24:47 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

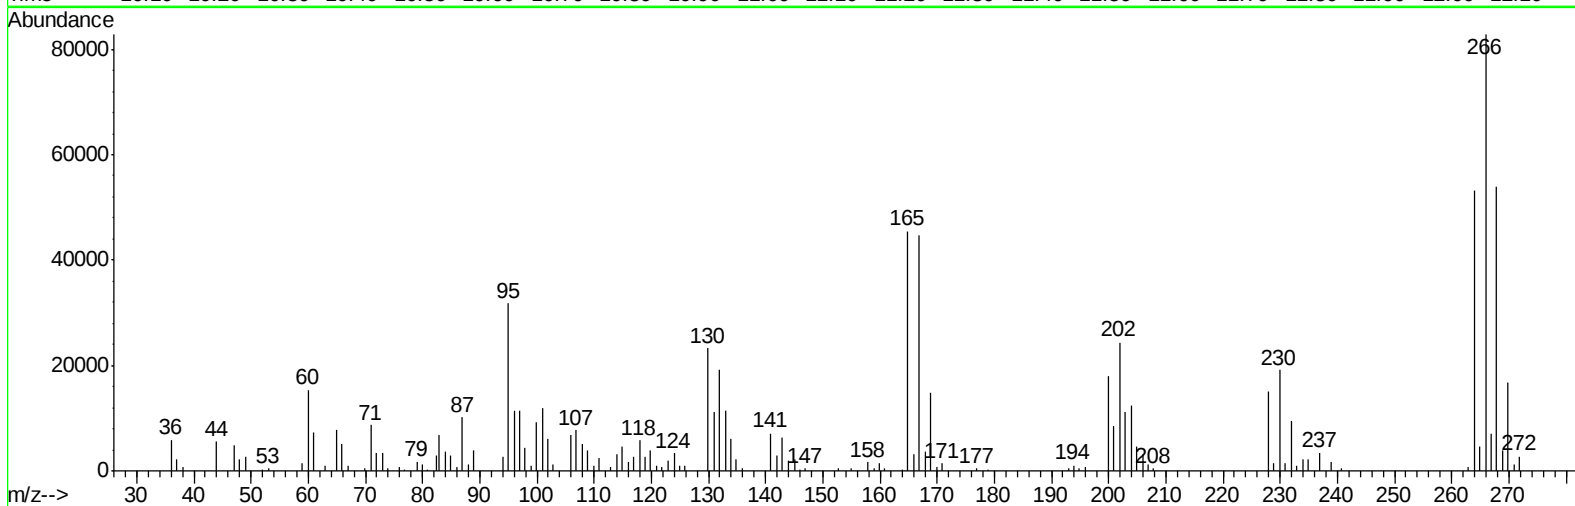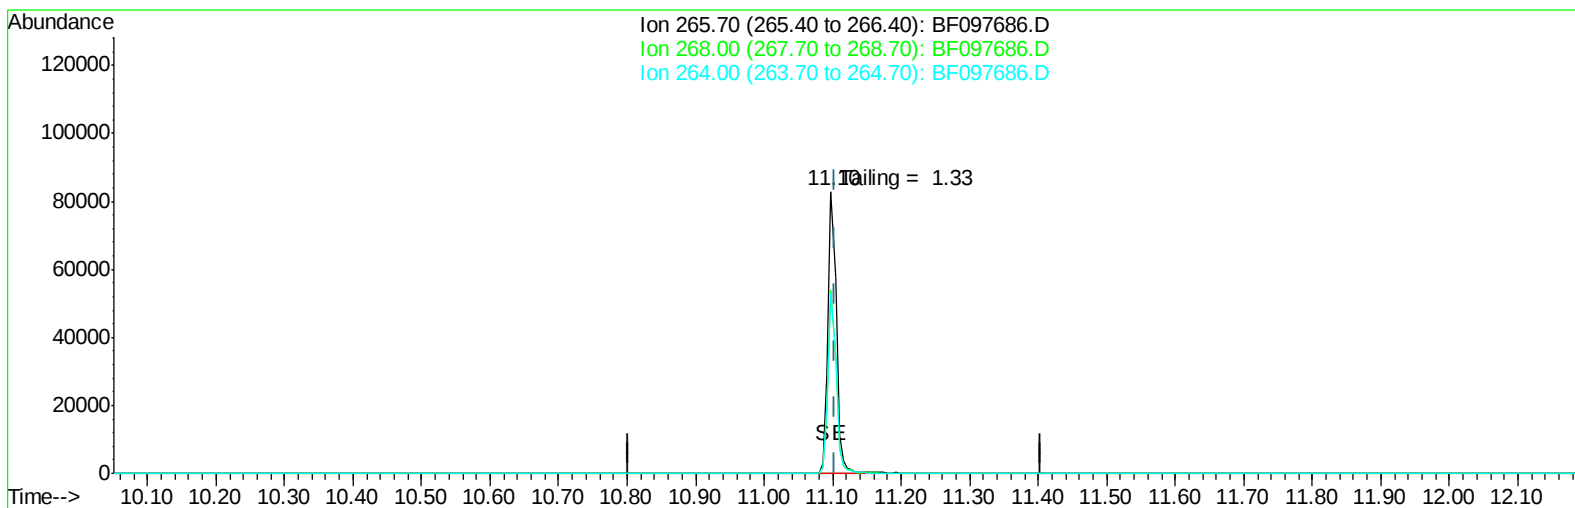

TIC: BF097686.D

(69) Pentachlorophenol (C)

11.098min (-0.006) 17984.89ng

response 68370

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.18
264.00	64.60	64.14
0.00	0.00	0.00