
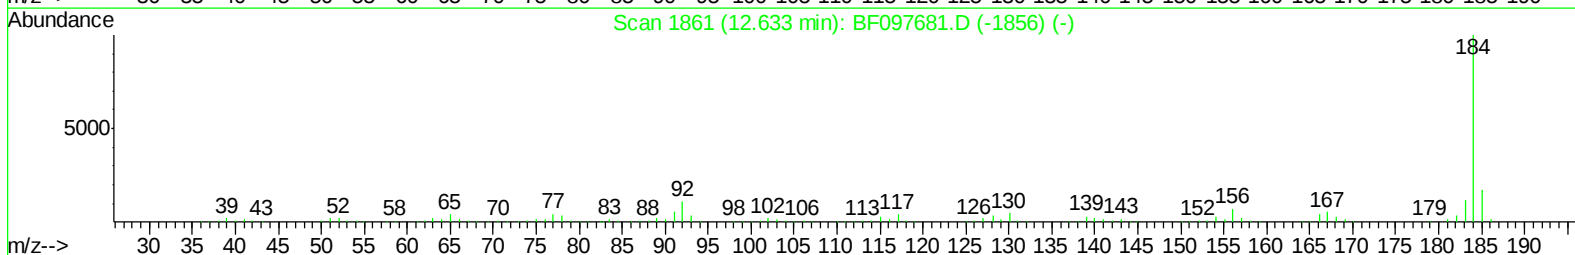
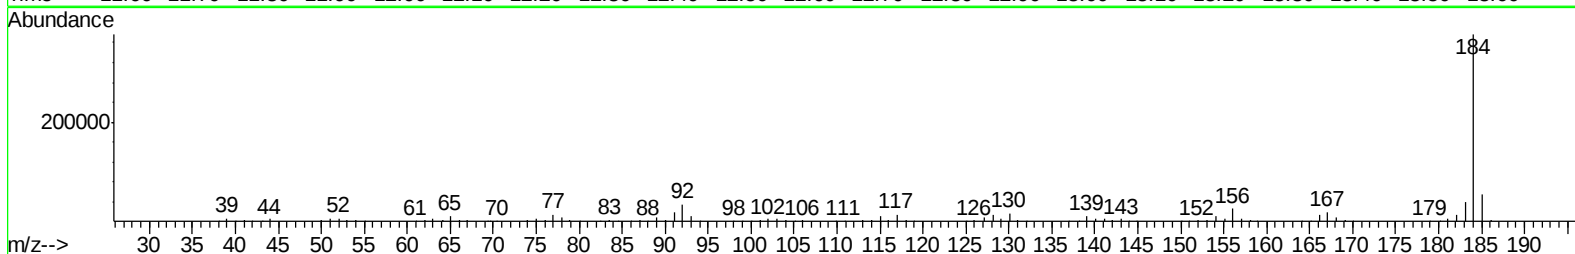


Data Path : Z:\HPCHEM1\BNA F\DATA\BF081517\
 Data File : BF097712.D
 Acq On : 16 Aug 2017 1:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 07:26:04 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 15 13:25:08 2017
 Response via : Initial Calibration

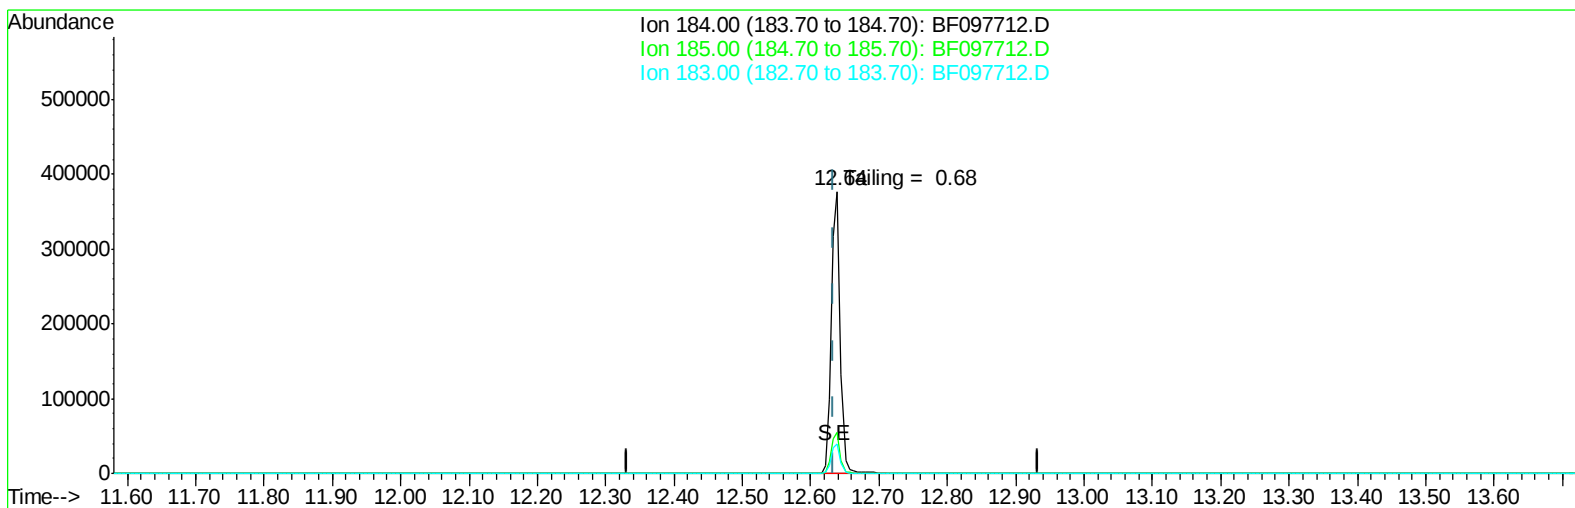

TIC: BF097712.D

(76) Benzidine




12.639min (+0.006) 34917.51ng

response 343460

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.51#
183.00	12.20	10.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF081517\
Data File : BF097712.D
Acq On : 16 Aug 2017 1:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 07:26:04 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 15 13:25:08 2017
Response via : Initial Calibration

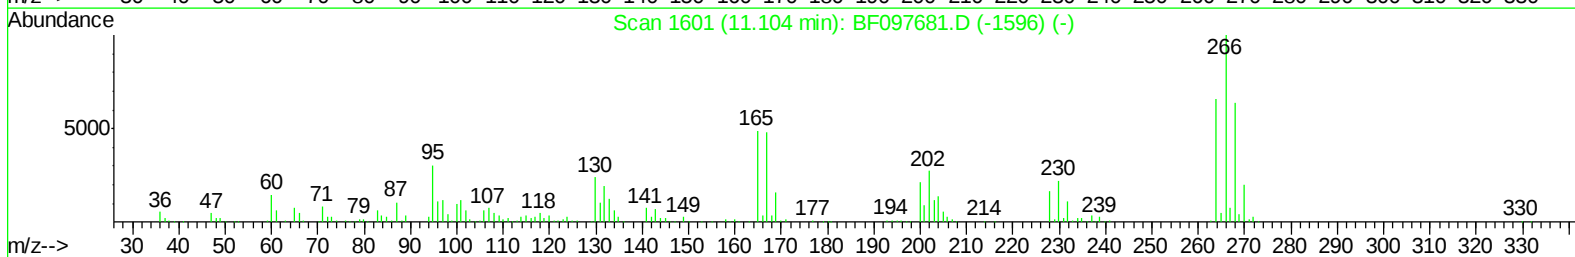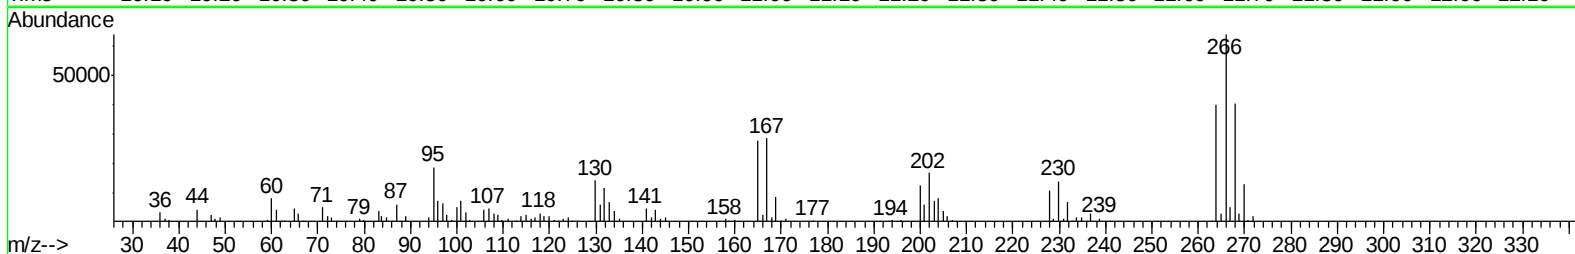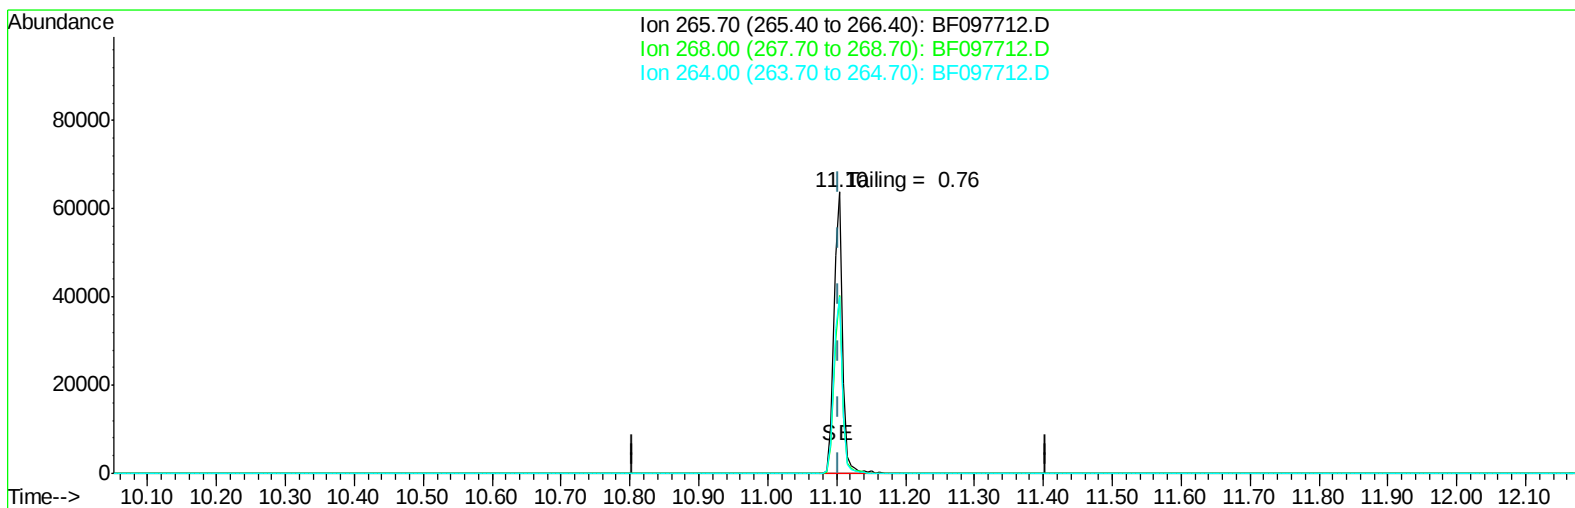

TIC: BF097712.D

(69) Pentachlorophenol (C)

11.104min (+0.000) 73307.02ng

response 54288

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.04
264.00	64.60	62.69
0.00	0.00	0.00