


Data Path : Z:\HPCHEM1\BNA_F\Data\BF081517\
 Data File : BF097677.D
 Acq On : 15 Aug 2017 8:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

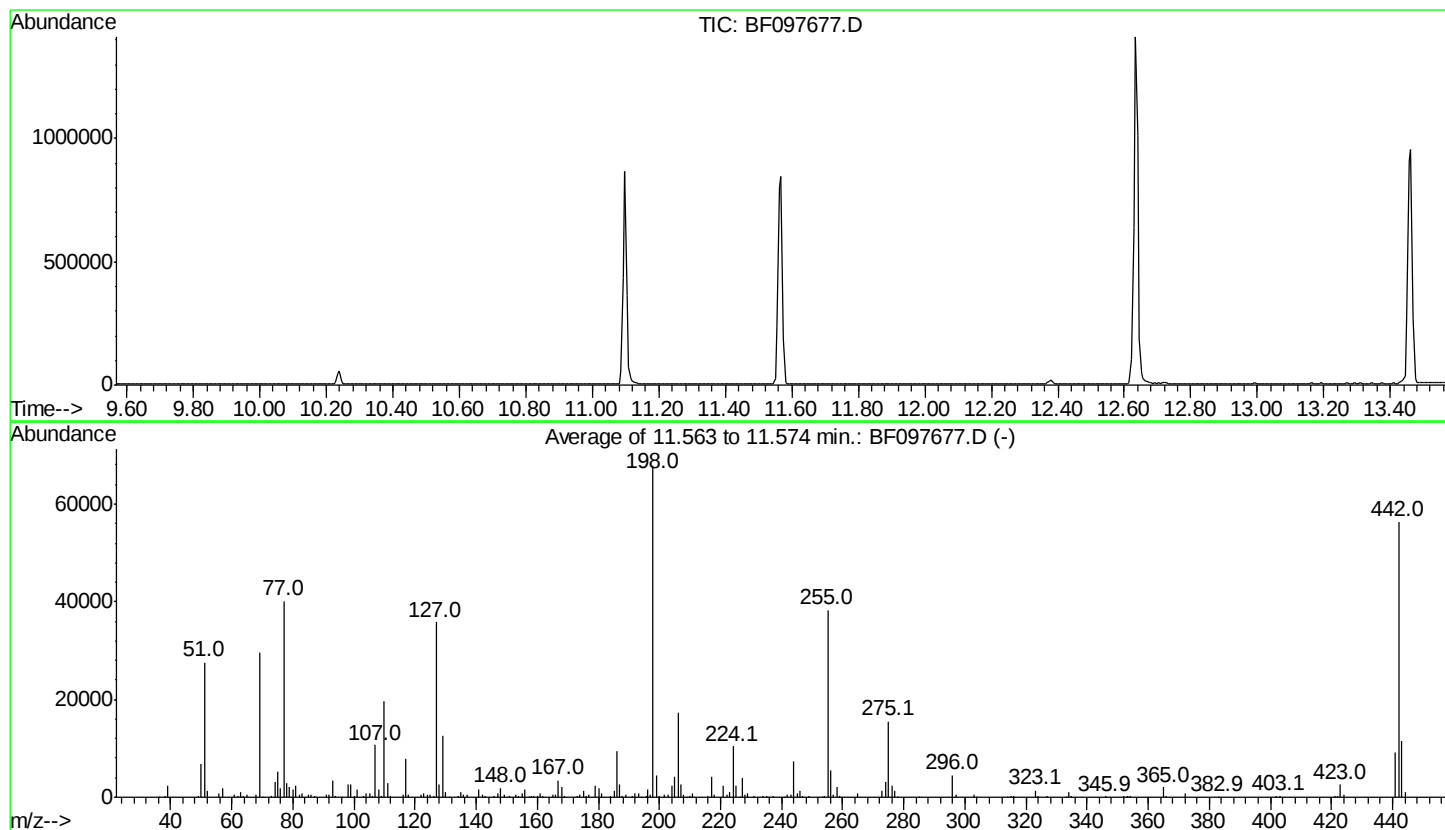

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1674

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	27634	PASS
68	69	0.00	2	1.5	448	PASS
69	198	0.00	100	43.6	29583	PASS
70	69	0.00	2	0.4	128	PASS
127	198	10	80	52.9	35869	PASS
197	198	0.00	2	0.9	627	PASS
198	198	100	100	100.0	67869	PASS
199	198	5	9	6.5	4410	PASS
275	198	10	60	22.8	15471	PASS
365	198	1	100	3.0	2062	PASS
441	442	0.01	24	16.2	9100	PASS
442	198	50	100	83.0	56346	PASS
443	442	15	24	20.5	11561	PASS