


Data Path : Z:\HPCHEM1\BNA F\Data\BF081517\
 Data File : BF097686.D
 Acq On : 15 Aug 2017 12:57
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

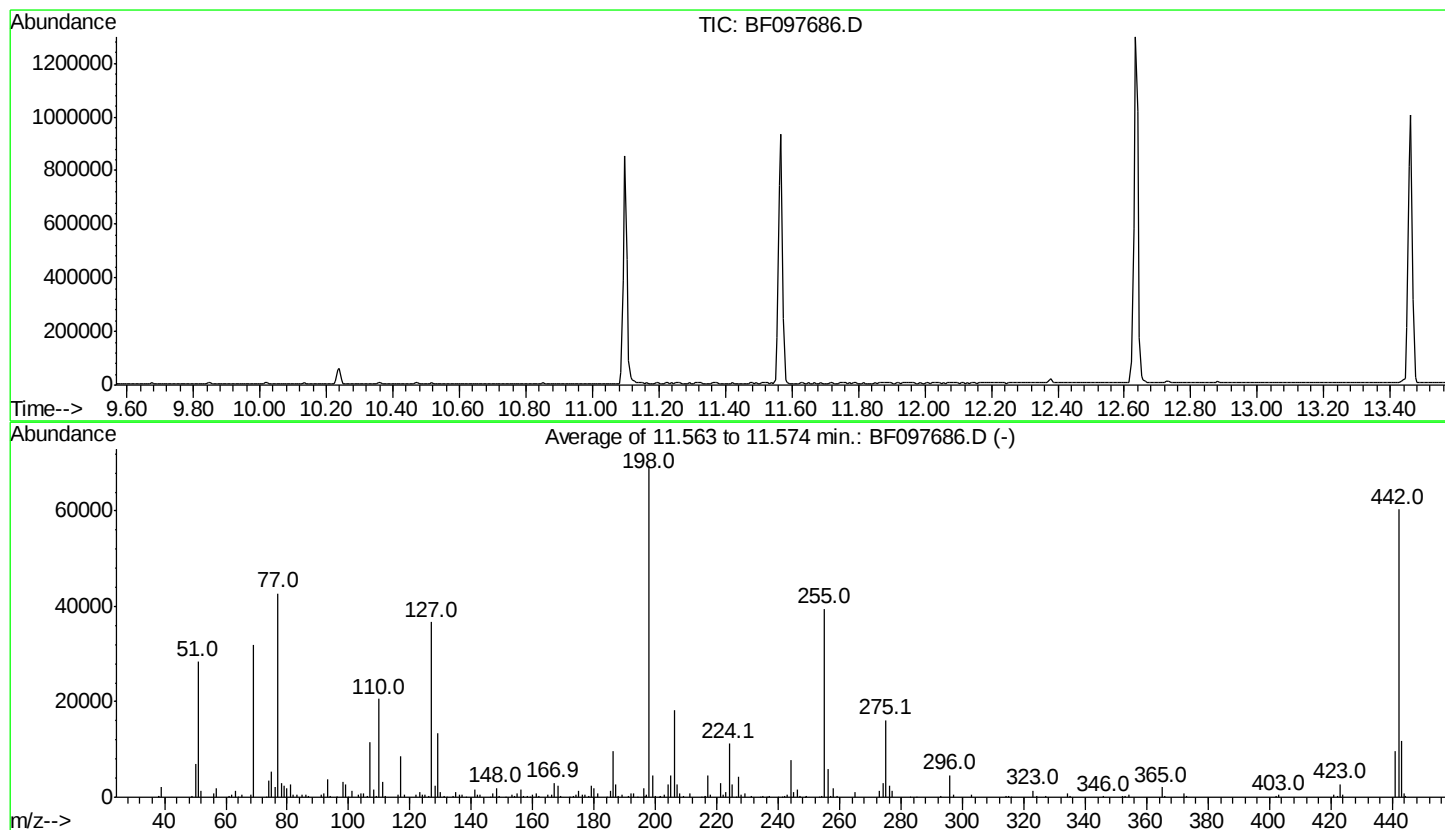

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.8	28380	PASS
68	69	0.00	2	1.6	524	PASS
69	198	0.00	100	46.1	32068	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.7	36644	PASS
197	198	0.00	2	0.8	564	PASS
198	198	100	100	100.0	69506	PASS
199	198	5	9	6.6	4599	PASS
275	198	10	60	23.4	16231	PASS
365	198	1	100	2.9	2043	PASS
441	442	0.01	24	15.9	9569	PASS
442	198	50	100	86.7	60288	PASS
443	442	15	24	19.5	11782	PASS