


Data Path : Z:\HPCHEM1\BNA F\Data\BF081517\
 Data File : BF097712.D
 Acq On : 16 Aug 2017 1:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

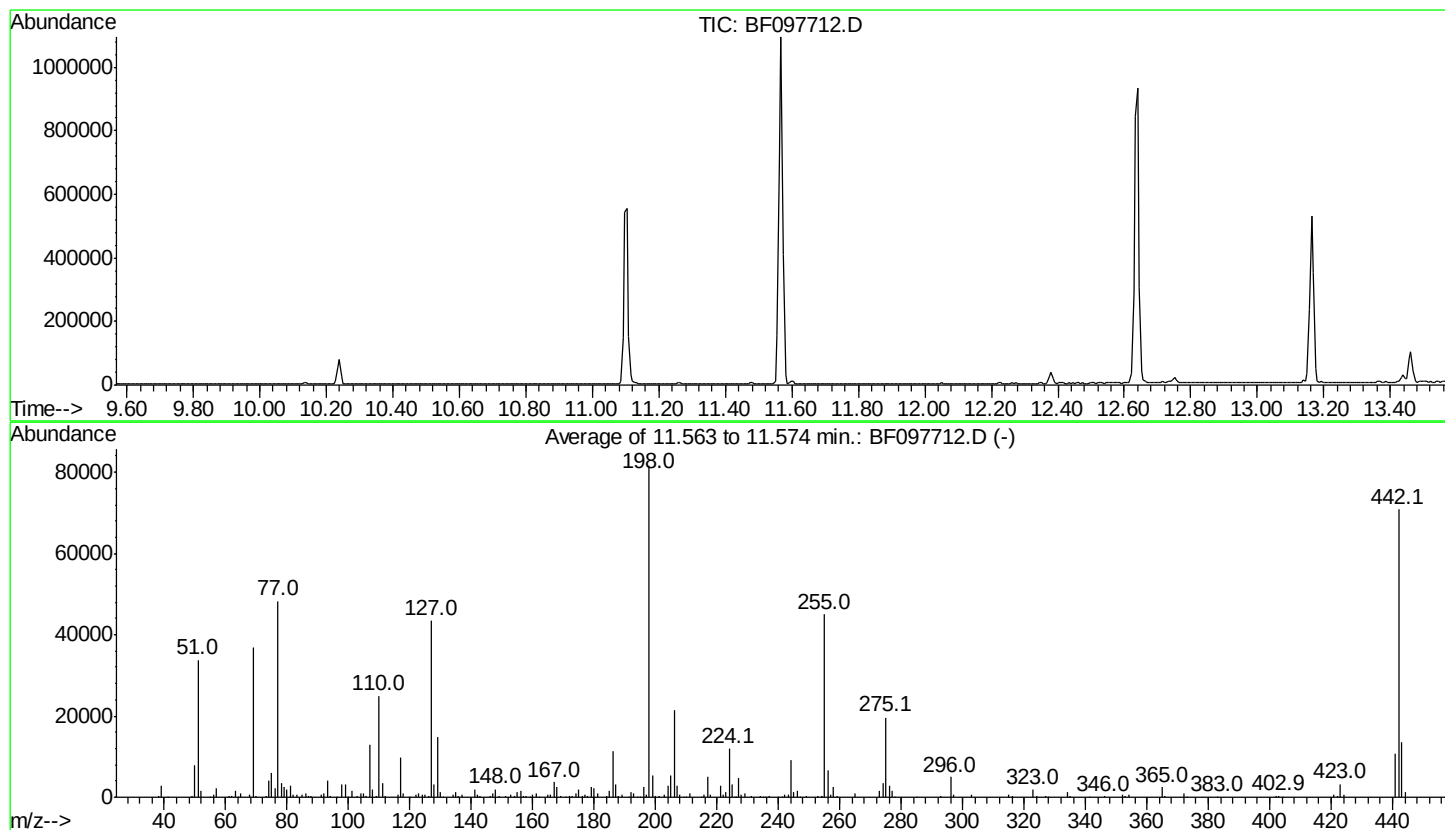

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	33851	PASS
68	69	0.00	2	1.6	600	PASS
69	198	0.00	100	45.1	36842	PASS
70	69	0.00	2	0.7	241	PASS
127	198	10	80	53.2	43434	PASS
197	198	0.00	2	0.6	529	PASS
198	198	100	100	100.0	81632	PASS
199	198	5	9	6.5	5295	PASS
275	198	10	60	24.0	19599	PASS
365	198	1	100	3.0	2410	PASS
441	442	0.01	24	15.3	10808	PASS
442	198	50	100	86.7	70768	PASS
443	442	15	24	19.1	13536	PASS