

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081518\
 Data File : BF108169.D
 Acq On : 15 Aug 2018 16:55
 Operator : JU/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 15 18:16:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.11	152	620468	40.00	ng	-0.16
2) Naphthalene-d8	11.57	136	7113	40.00	ng	-0.16
3) Acenaphthene-d10	14.79	164	588	40.00	ng	-0.11
4) Phenanthrene-d10	14.75	188	266	40.00	ng	-0.34
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.93
9) Perylene-d12	0.00	264	0	0.00	ng	-34.56
Target Compounds						Ovalue
5) DDE	0.00	246	0	N.D.		
6) DDD	10.39	235	13375	19.489	ng	# 1
7) DDT	10.87	235	301	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081518\
Data File : BF108169.D
Acq On : 15 Aug 2018 16:55
Operator : JU/SJ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 15 18:16:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration


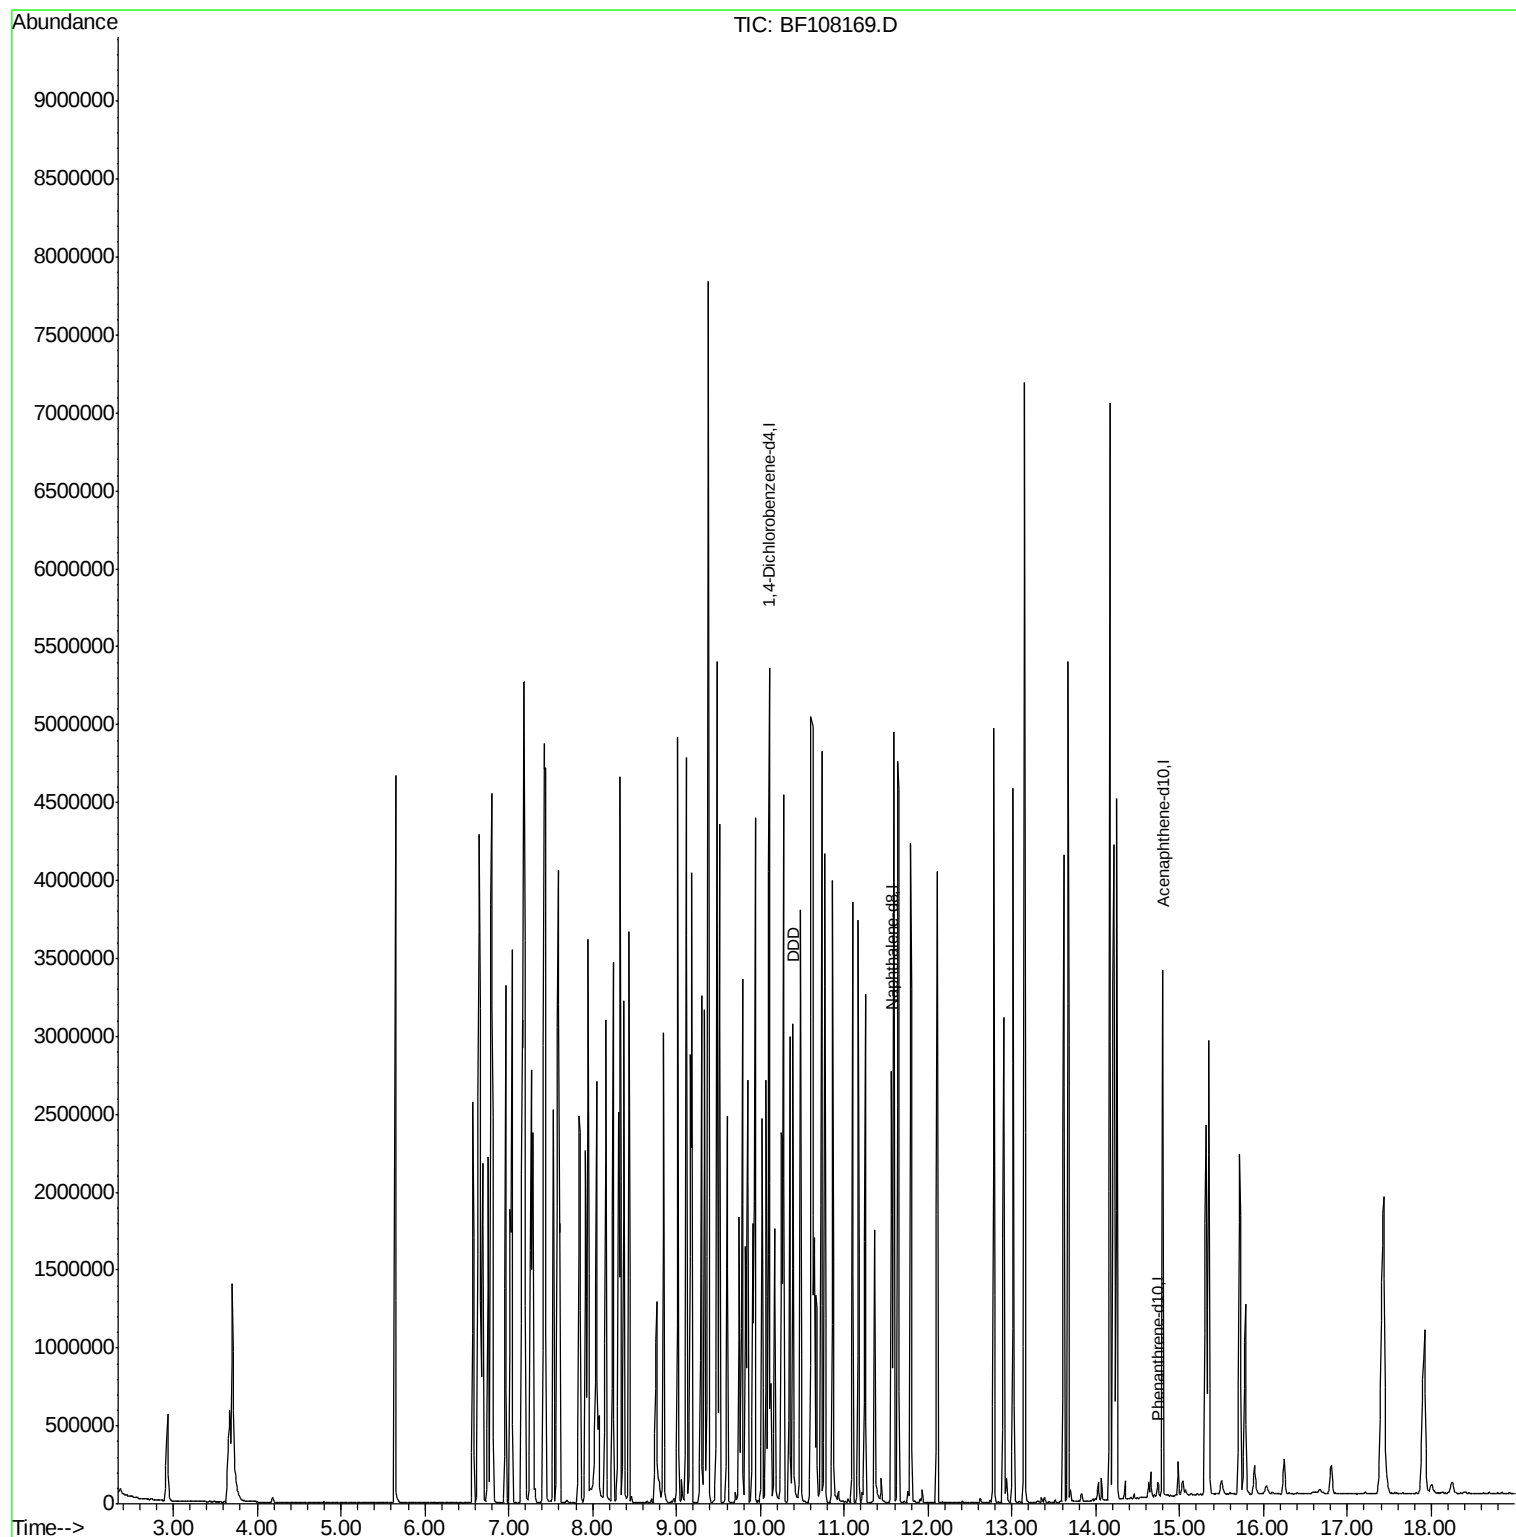


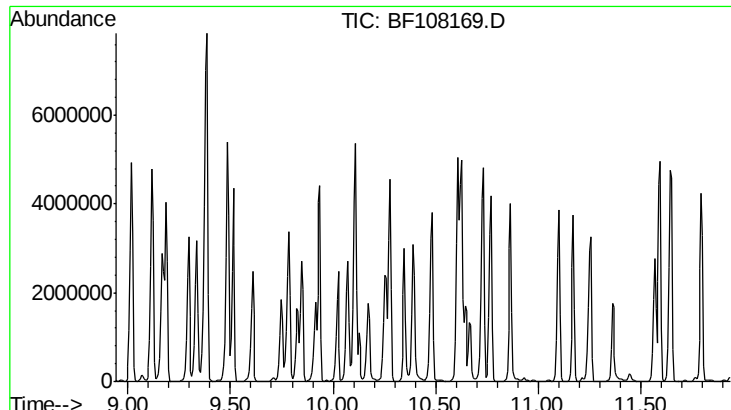

#5
DDE
Concen: N.D.
Expected RT: 10.44 min
Lab File: BF108169.D
Acq: 15 Aug 2018 16:55




Instrument :
BNA_F
ClientSampleId :


Tot Ion: 246
Sig Exp Ratio
246 100
248 1793.6
318 201.9
176 4805.3

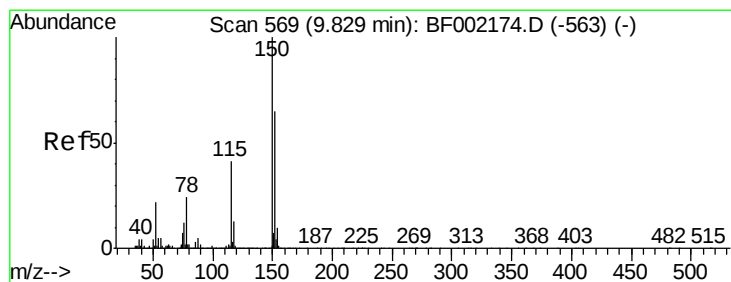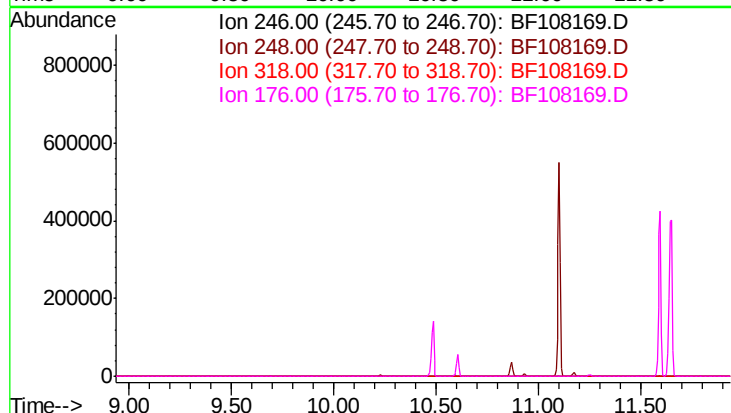

#6
DDD
Concen: 19.489 ng
RT: 10.39 min Scan# 1369
Delta R.T. -0.44 min
Lab File: BF108169.D
Acq: 15 Aug 2018 16:55

Tgt Ion:235 Resp: 13375
Ion Ratio Lower Upper
235 100
237 21.0 4800.0 7200.0#
165 0.0 4800.0 7200.0#

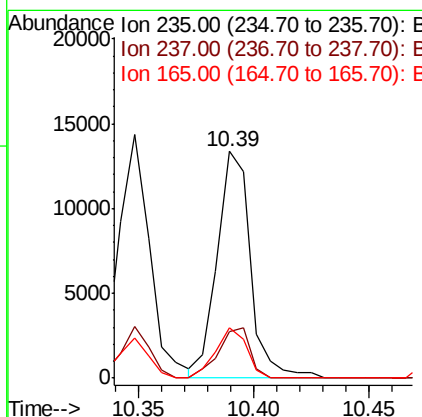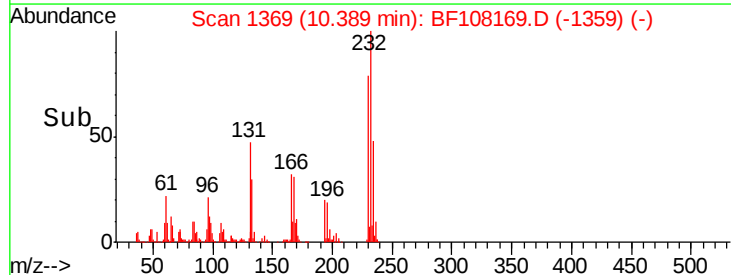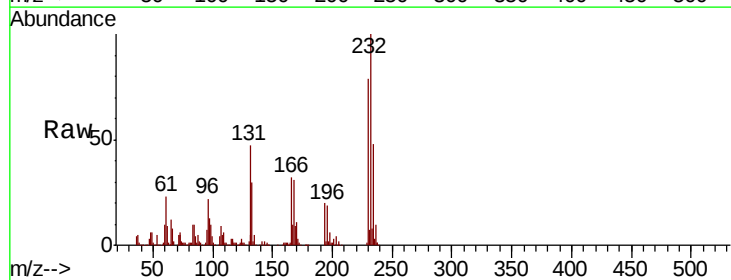

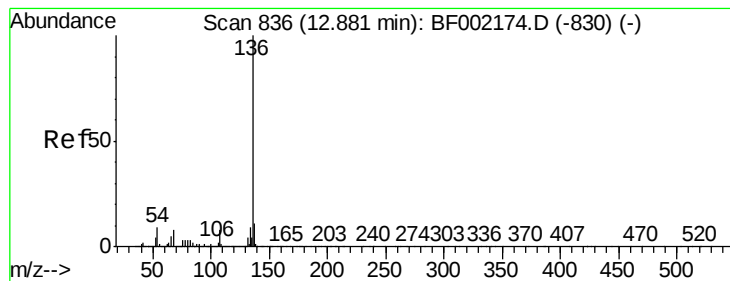

#7

DDT

Concen: Below Cal

RT: 10.87 min Scan# 1451

Delta R.T. -0.32 min


Lab File: BF108169.D

Acq: 15 Aug 2018 16:55

Instrument :

BNA_F

ClientSampleId :

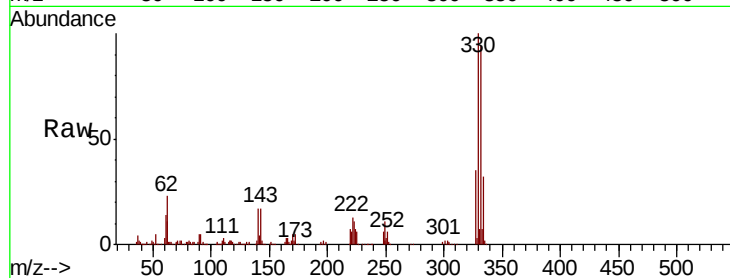

Tot Ion:	235	Resp:	301
Ion	Ratio	Lower	Upper
235	100		
237	168.8	0.0	0.0#
165	0.0	0.2	0.2#

