

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081518\
 Data File : BF108170.D
 Acq On : 15 Aug 2018 17:22
 Operator : JU/SJ
 Sample : PB112068BS
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 15 18:16:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.10	152	485869	40.00	ng	-0.16
2) Naphthalene-d8	11.57	136	5408	40.00	ng	-0.16
3) Acenaphthene-d10	14.80	164	699	40.00	ng	-0.11
4) Phenanthrene-d10	14.75	188	220	40.00	ng	-0.34
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.93
9) Perylene-d12	0.00	264	0	0.00	ng	-34.56
Target Compounds						Ovalue
5) DDE	0.00	246	0	N.D.		
6) DDD	10.39	235	10698	18.848	ng	# 1
7) DDT	10.87	235	269	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF081518\
Data File : BF108170.D
Acq On : 15 Aug 2018 17:22
Operator : JU/SJ
Sample : PB112068BS
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 15 18:16:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

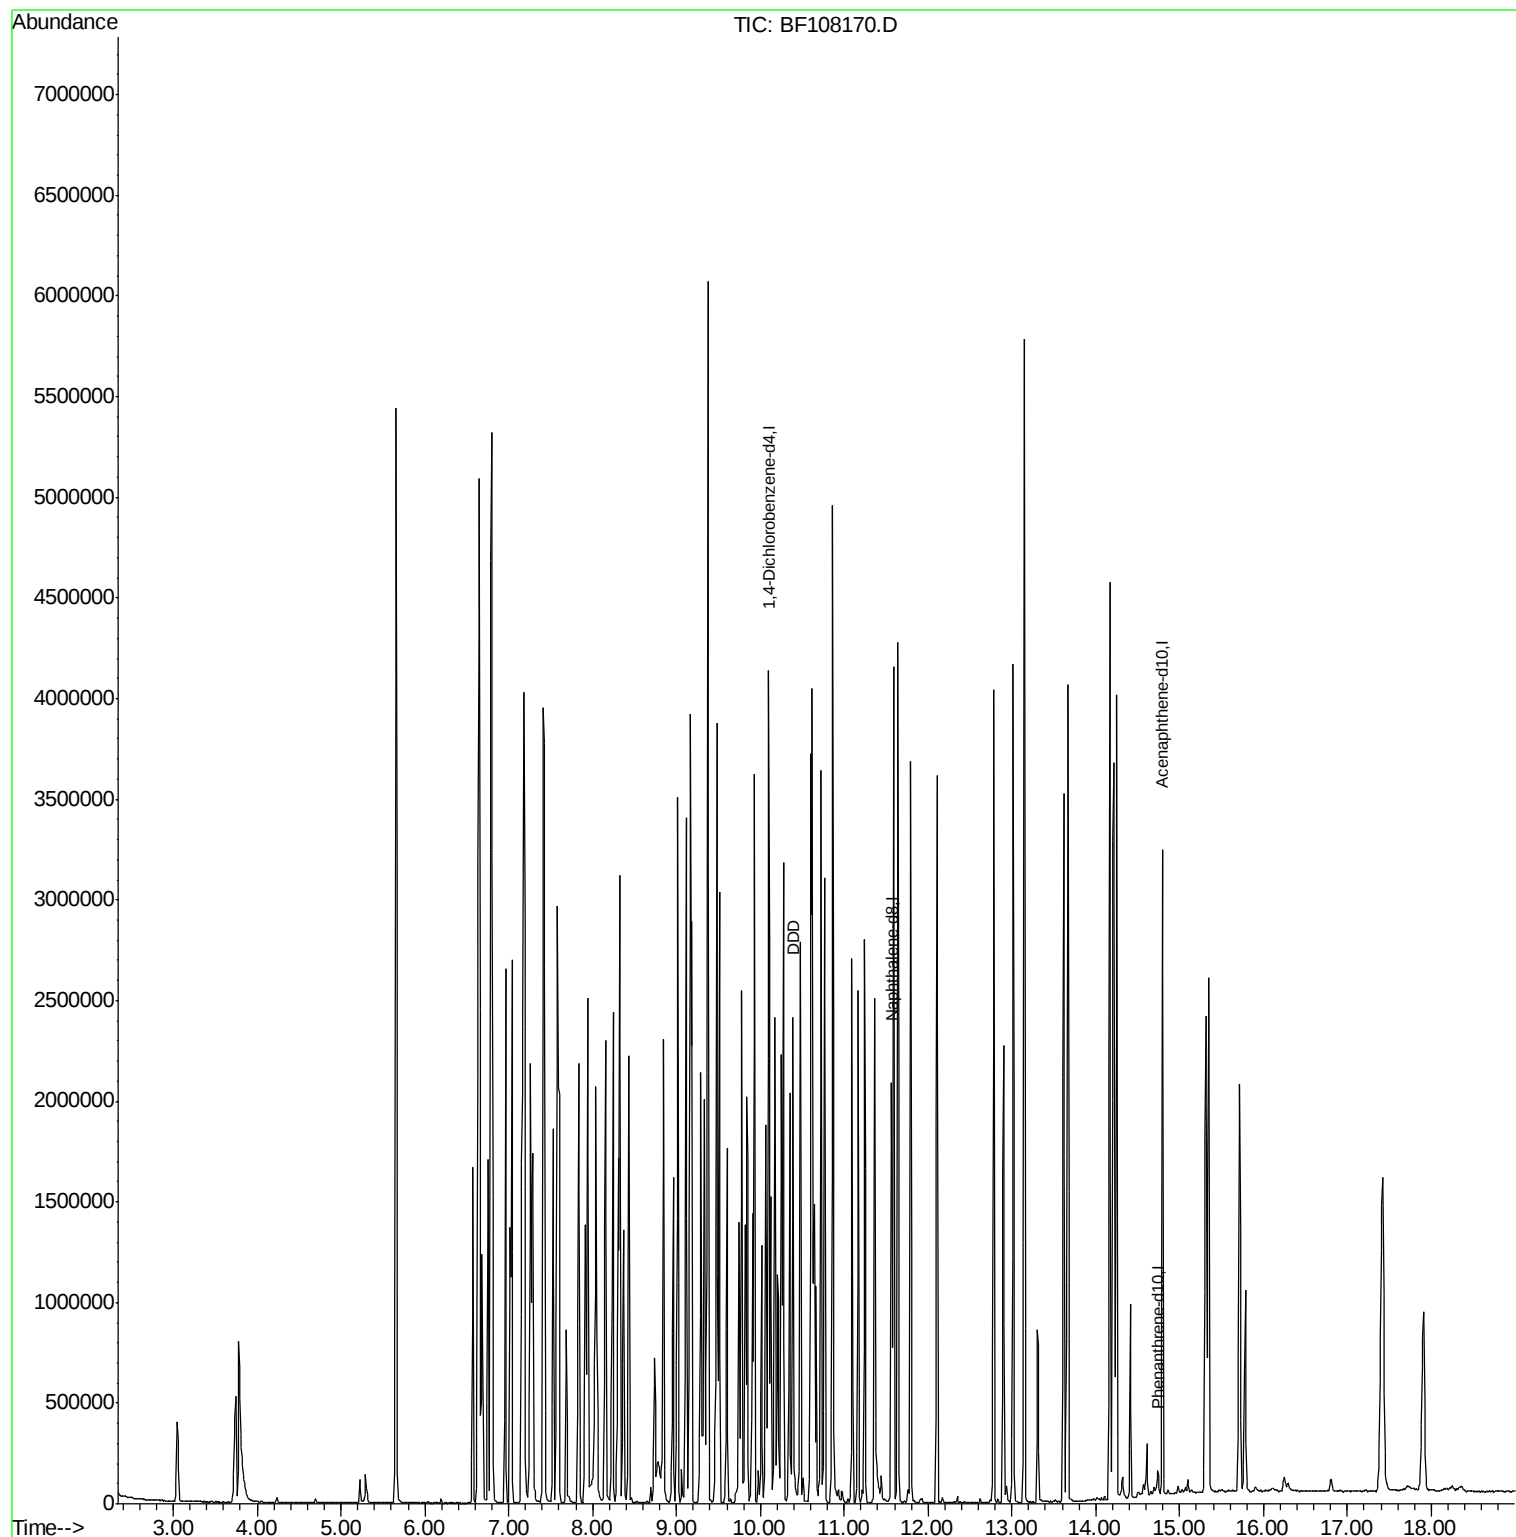

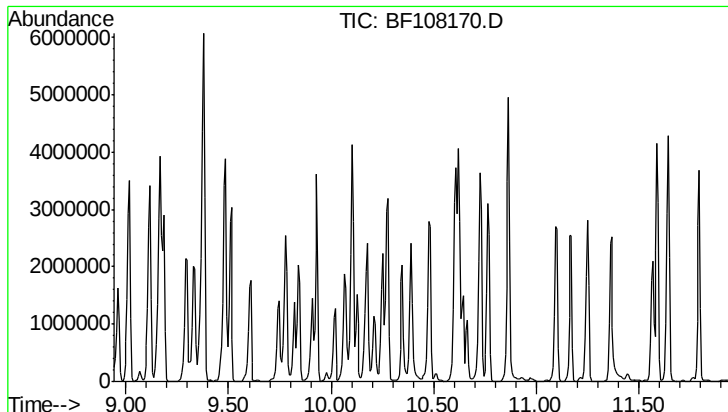

#5

DDE

Concen: N.D.

Expected RT: 10.44 min

Lab File: BF108170.D

Acq: 15 Aug 2018 17:22

Instrument :

BNA_F

ClientSampleId :

Tot Ion: 246



Sig Exp Ratio

246 100

248 1793.6

318 201.9

176 4805.3

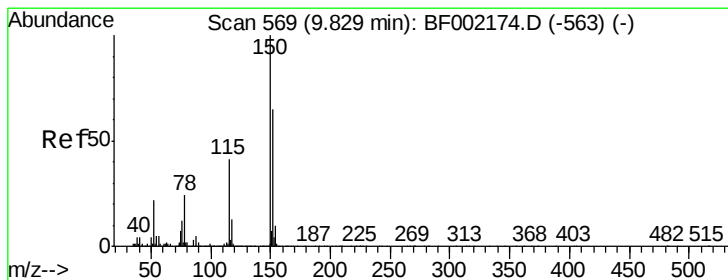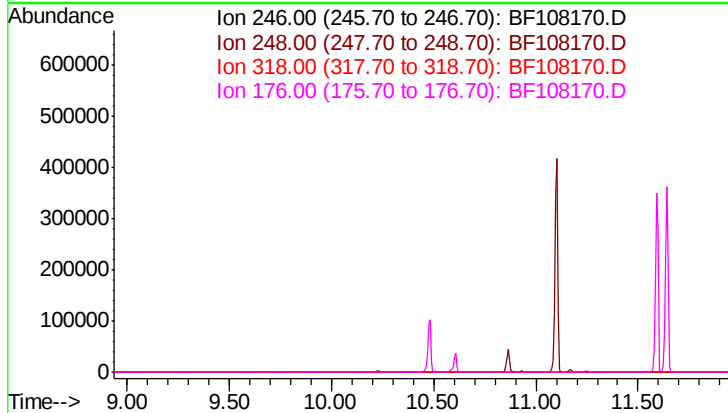

#6

DDD

Concen: 18.848 ng

RT: 10.39 min Scan# 1369

Delta R.T. -0.44 min

Lab File: BF108170.D

Acq: 15 Aug 2018 17:22




Tgt Ion:235 Resp: 10698


Ion Ratio Lower Upper

235 100

237 18.5 4800.0 7200.0#

165 0.0 4800.0 7200.0#

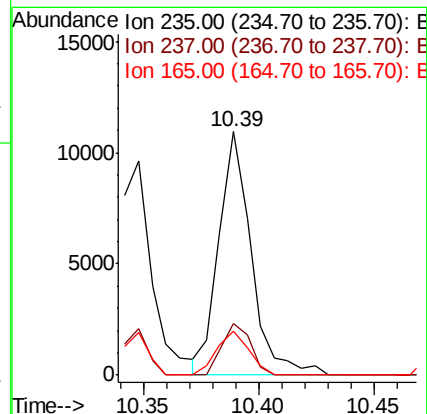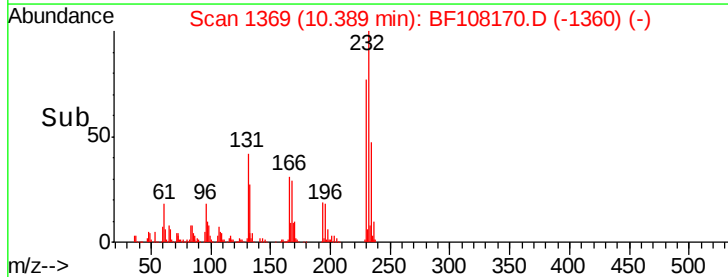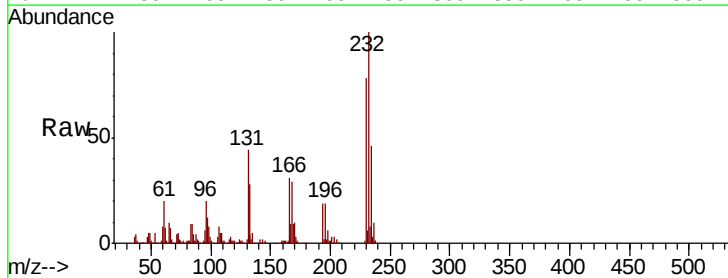

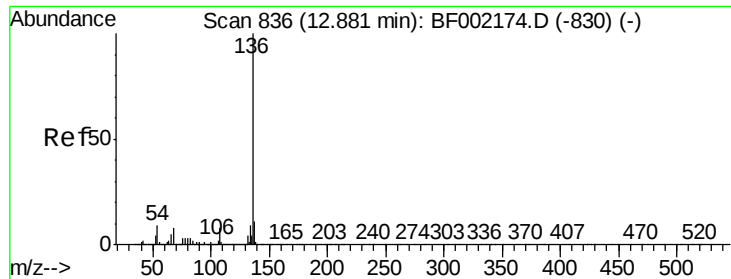

#7

DDT

Concen: Below Cal

RT: 10.87 min Scan# 1450

Delta R.T. -0.33 min

Lab File: BF108170.D

Acq: 15 Aug 2018 17:22

Instrument :

BNA_F

ClientSampleId :



Tot Ion:235 Resp: 269

Ion Ratio Lower Upper

235 100

237 153.9 0.0 0.0#

165 0.0 0.2 0.2#

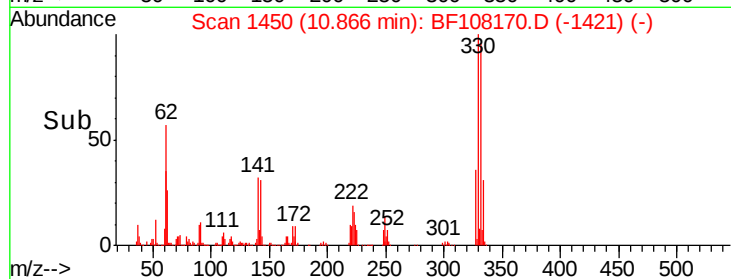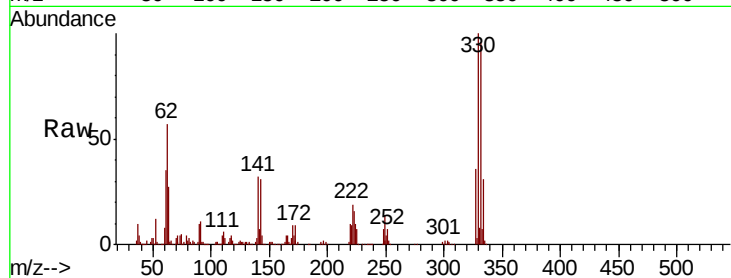

Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

