
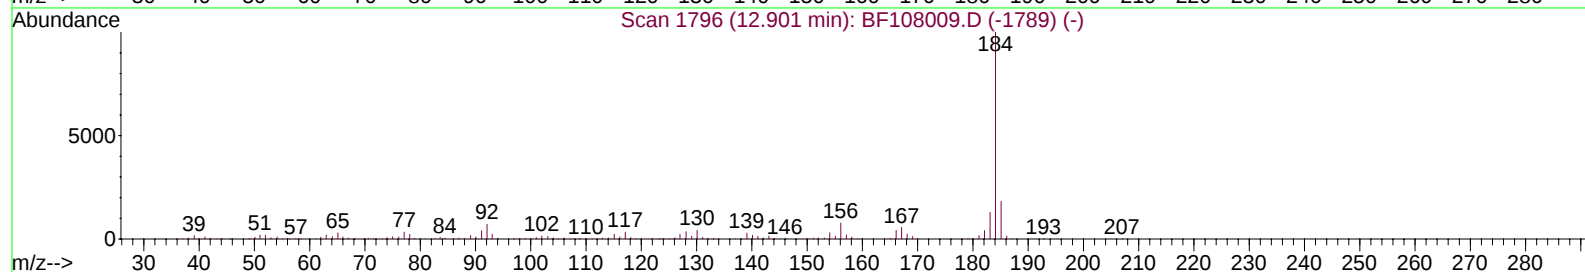
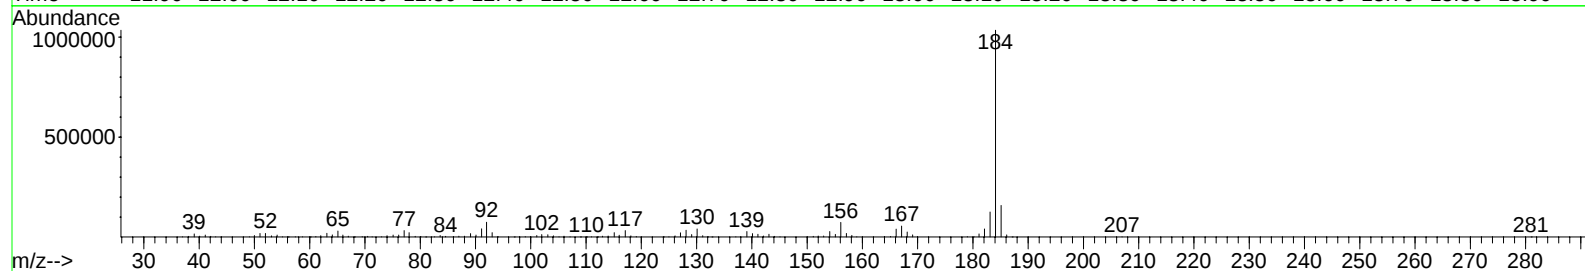


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081518\  
Data File   : BF108168.D  
Acq On      : 15 Aug 2018   16:28  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Aug 15 19:21:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

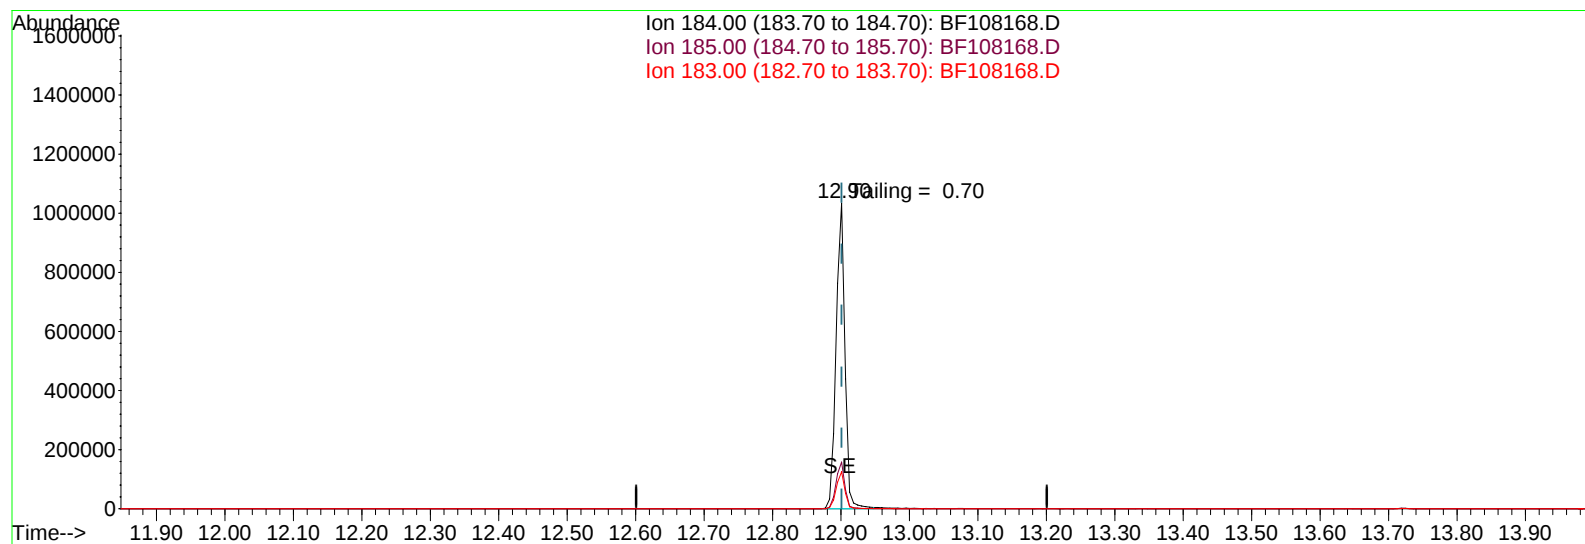

TIC: BF108168.D

(76) Benzidine




12.901min (+0.000) 98082.17ng

response 938135

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.29
183.00	11.60	12.09
0.00	0.00	0.00

```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF081518\  
Data File   : BF108168.D  
Acq On      : 15 Aug 2018   16:28  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Aug 15 19:21:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

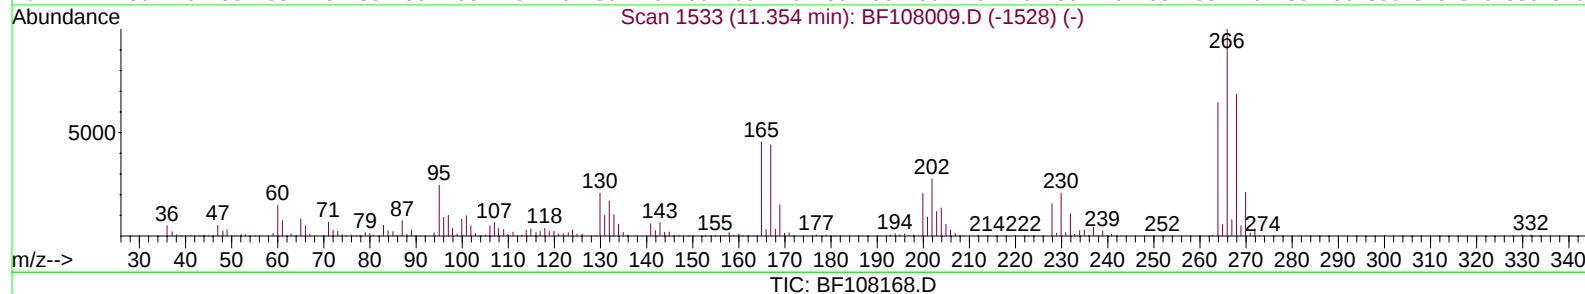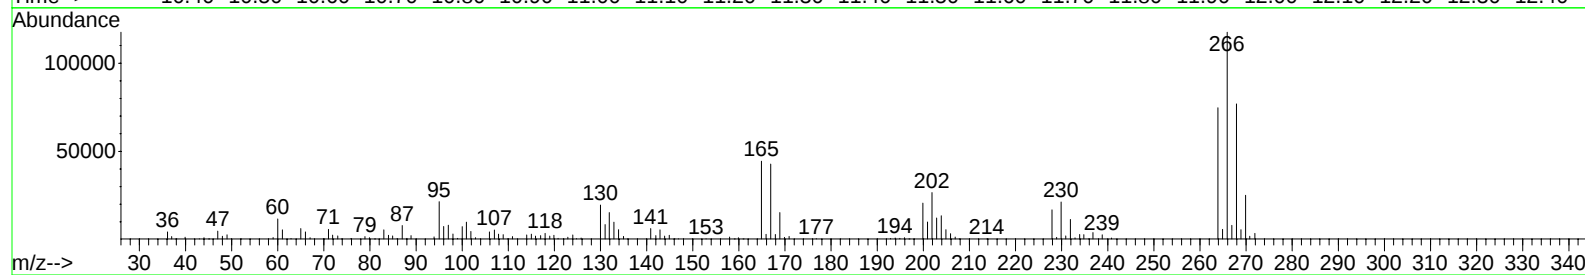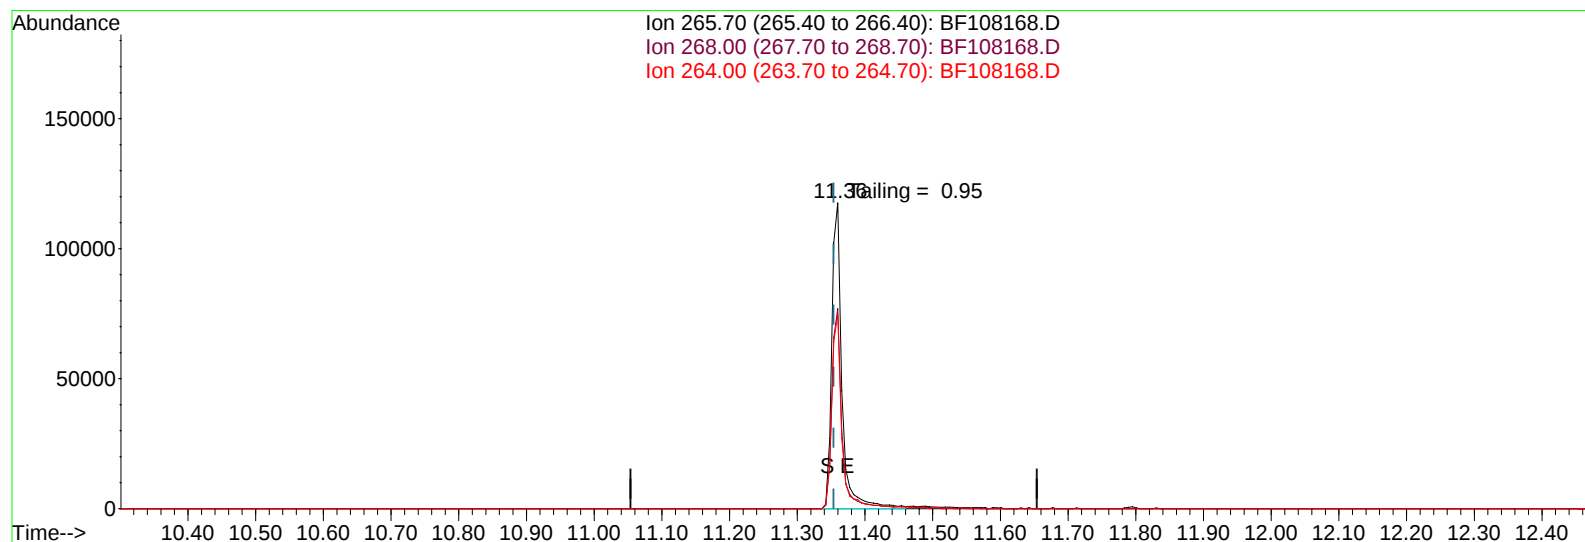

(69) Pentachlorophenol (C)

11.360min (+0.006) 25940.26ng

```
response 123228
```

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.44
264.00	61.90	63.58
0.00	0.00	0.00