


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081518\
 Data File : BF108168.D
 Acq On : 15 Aug 2018 16:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 08 12:24:24 2018

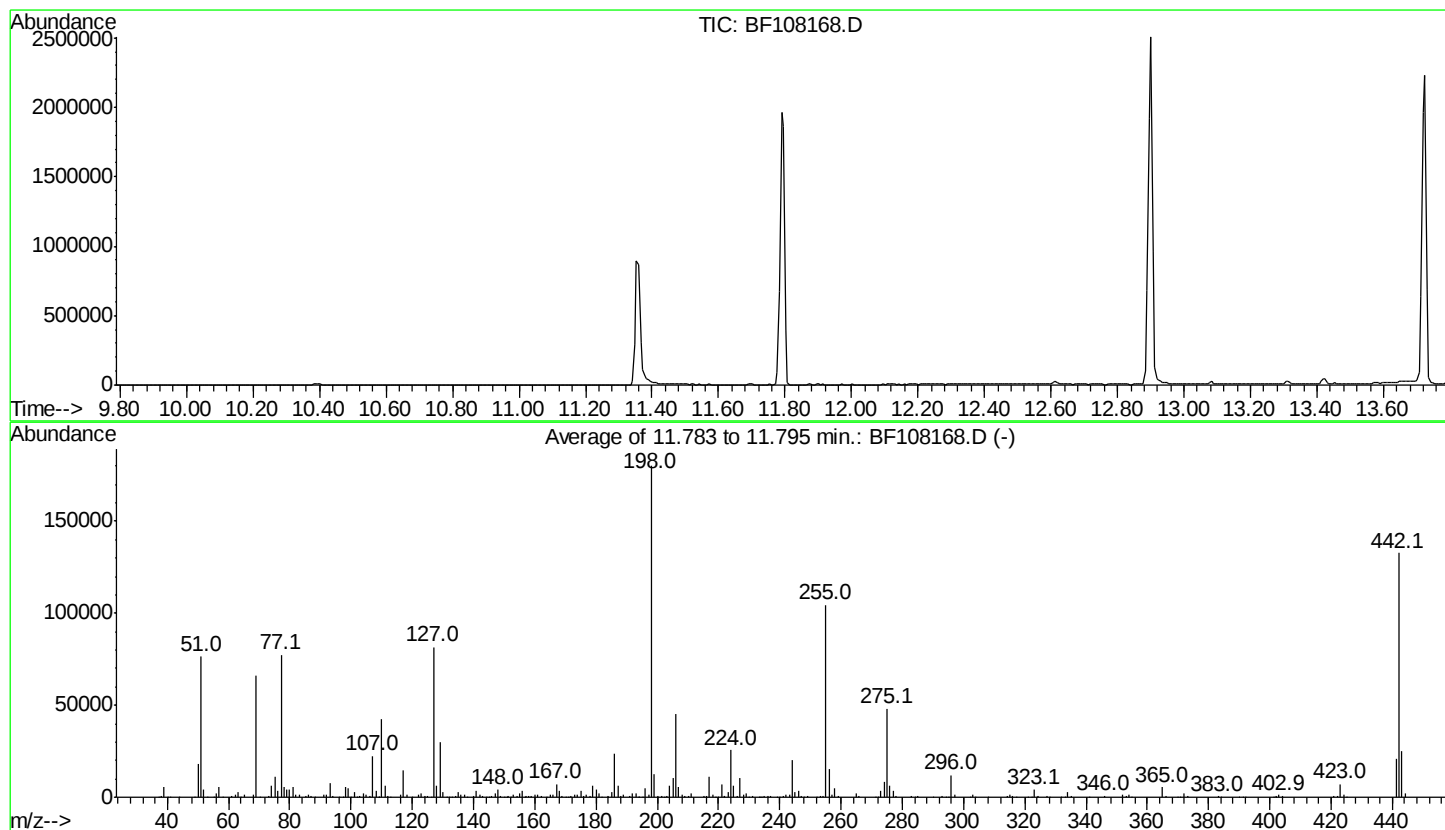

AutoFind: Scans 1606, 1607, 1608; Background Corrected with Scan 1601

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	76344	PASS
68	69	0.00	2	1.6	1079	PASS
69	198	0.00	100	36.8	66256	PASS
70	69	0.00	2	0.5	324	PASS
127	198	10	80	45.3	81616	PASS
197	198	0.00	2	0.8	1445	PASS
198	198	100	100	100.0	180208	PASS
199	198	5	9	6.9	12402	PASS
275	198	10	60	26.7	48160	PASS
365	198	1	100	3.0	5350	PASS
441	198	0.01	100	11.5	20673	PASS
442	198	50	100	73.7	132858	PASS
443	442	15	24	18.8	24927	PASS