


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081519\  
 Data File : BF116270.D  
 Acq On : 15 Aug 2019 10:38  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF073019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 19 06:03:31 2019

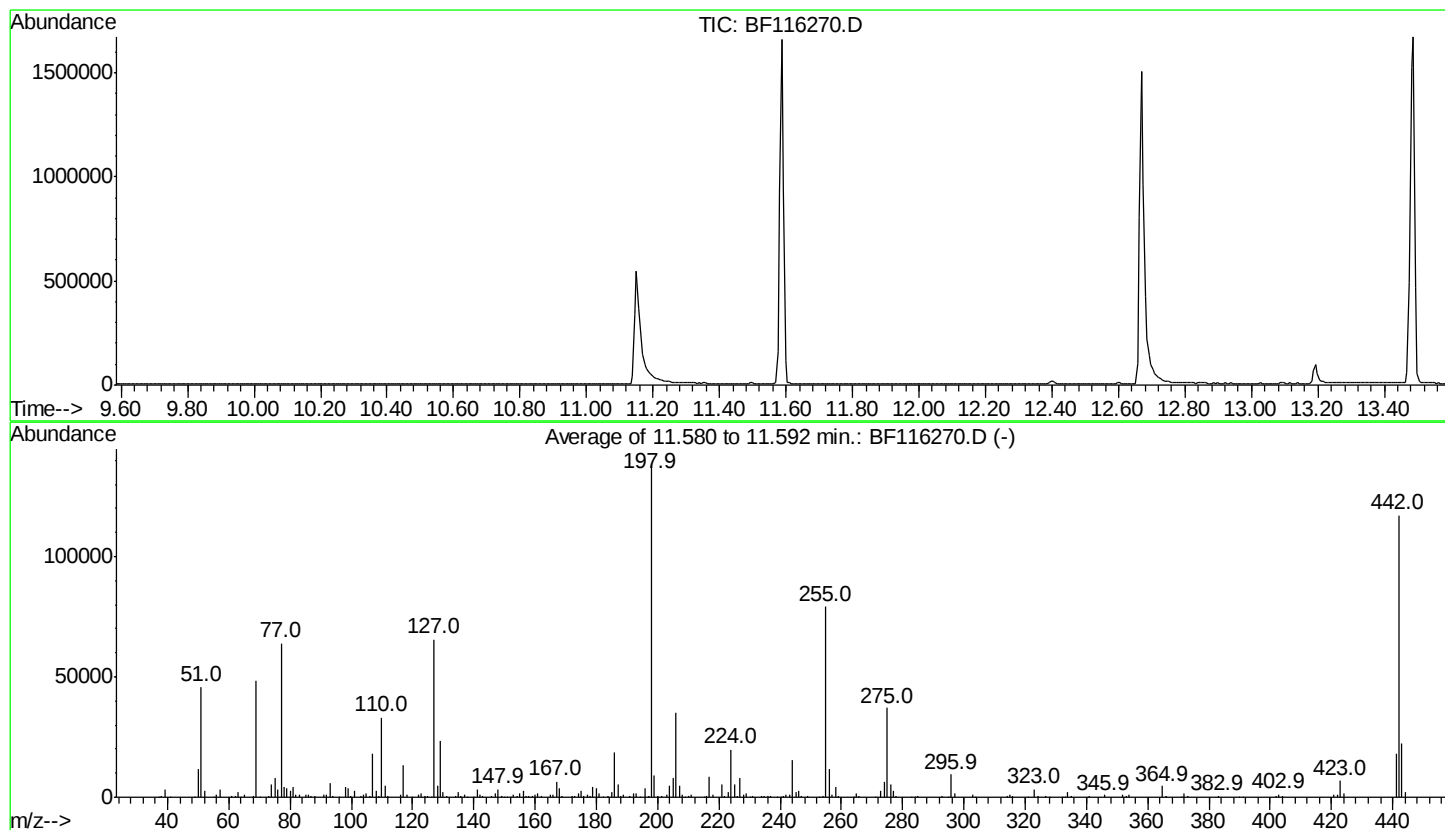

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 33.3         | 45899      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 795        | PASS                |
| 69             | 198             | 0.00            | 100             | 35.1         | 48360      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 105        | PASS                |
| 127            | 198             | 10              | 80              | 47.5         | 65472      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 582        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 137813     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 9062       | PASS                |
| 275            | 198             | 10              | 60              | 26.9         | 37090      | PASS                |
| 365            | 198             | 1               | 100             | 3.4          | 4736       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.2         | 18249      | PASS                |
| 442            | 198             | 50              | 100             | 84.9         | 117048     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 22348      | PASS                |