


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081519\
 Data File : BF116282.D
 Acq On : 15 Aug 2019 17:06
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 19 06:03:31 2019

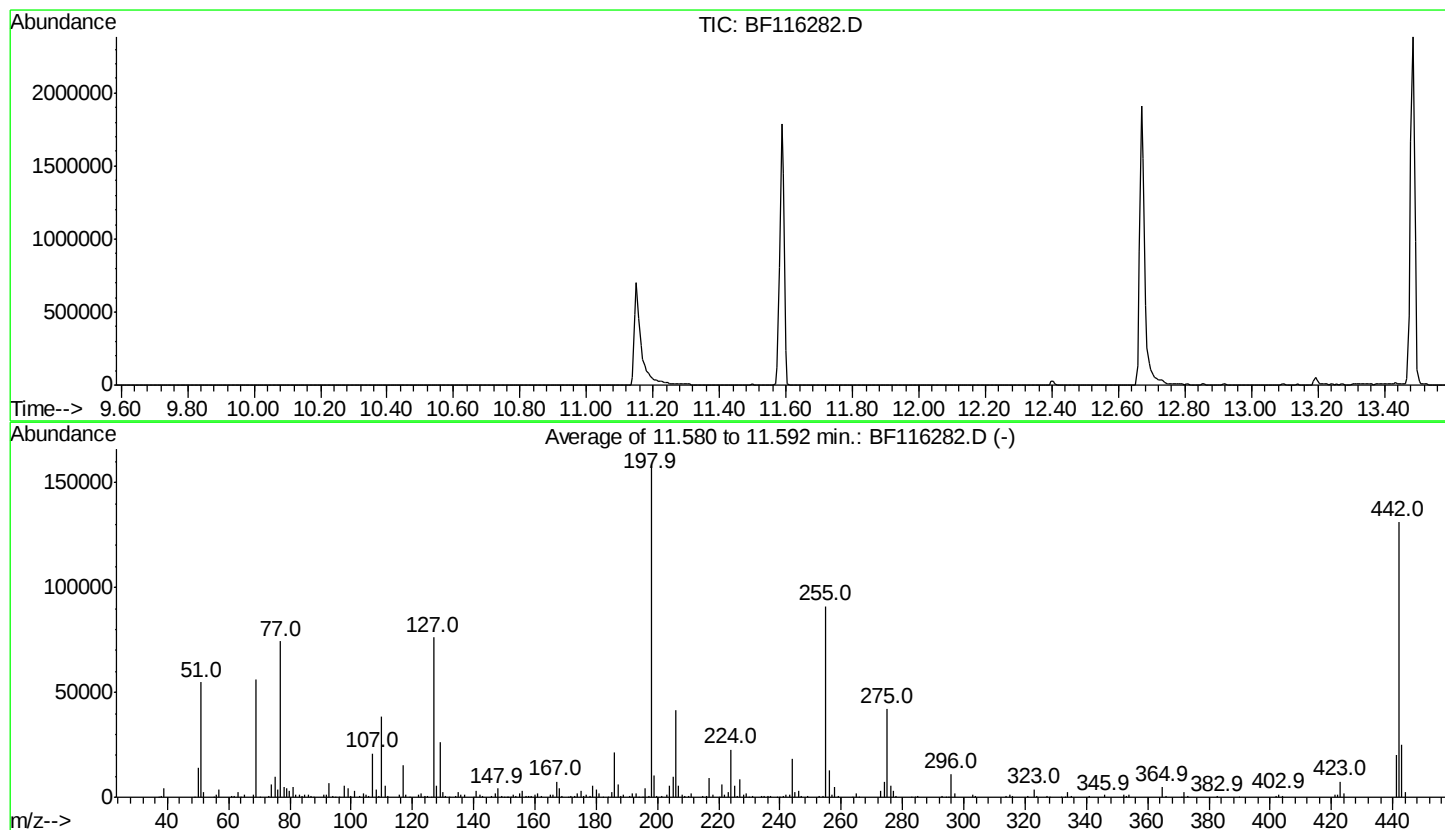

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	54805	PASS
68	69	0.00	2	1.7	971	PASS
69	198	0.00	100	35.5	56152	PASS
70	69	0.00	2	0.3	185	PASS
127	198	10	80	48.2	76250	PASS
197	198	0.00	2	0.5	835	PASS
198	198	100	100	100.0	158130	PASS
199	198	5	9	6.7	10532	PASS
275	198	10	60	26.8	42344	PASS
365	198	1	100	3.2	5044	PASS
441	198	0.01	100	12.9	20433	PASS
442	198	50	100	83.2	131501	PASS
443	442	15	24	19.2	25225	PASS