


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081522\  
 Data File : BF129781.D  
 Acq On : 15 Aug 2022 15:25  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081422.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 15 02:28:31 2022

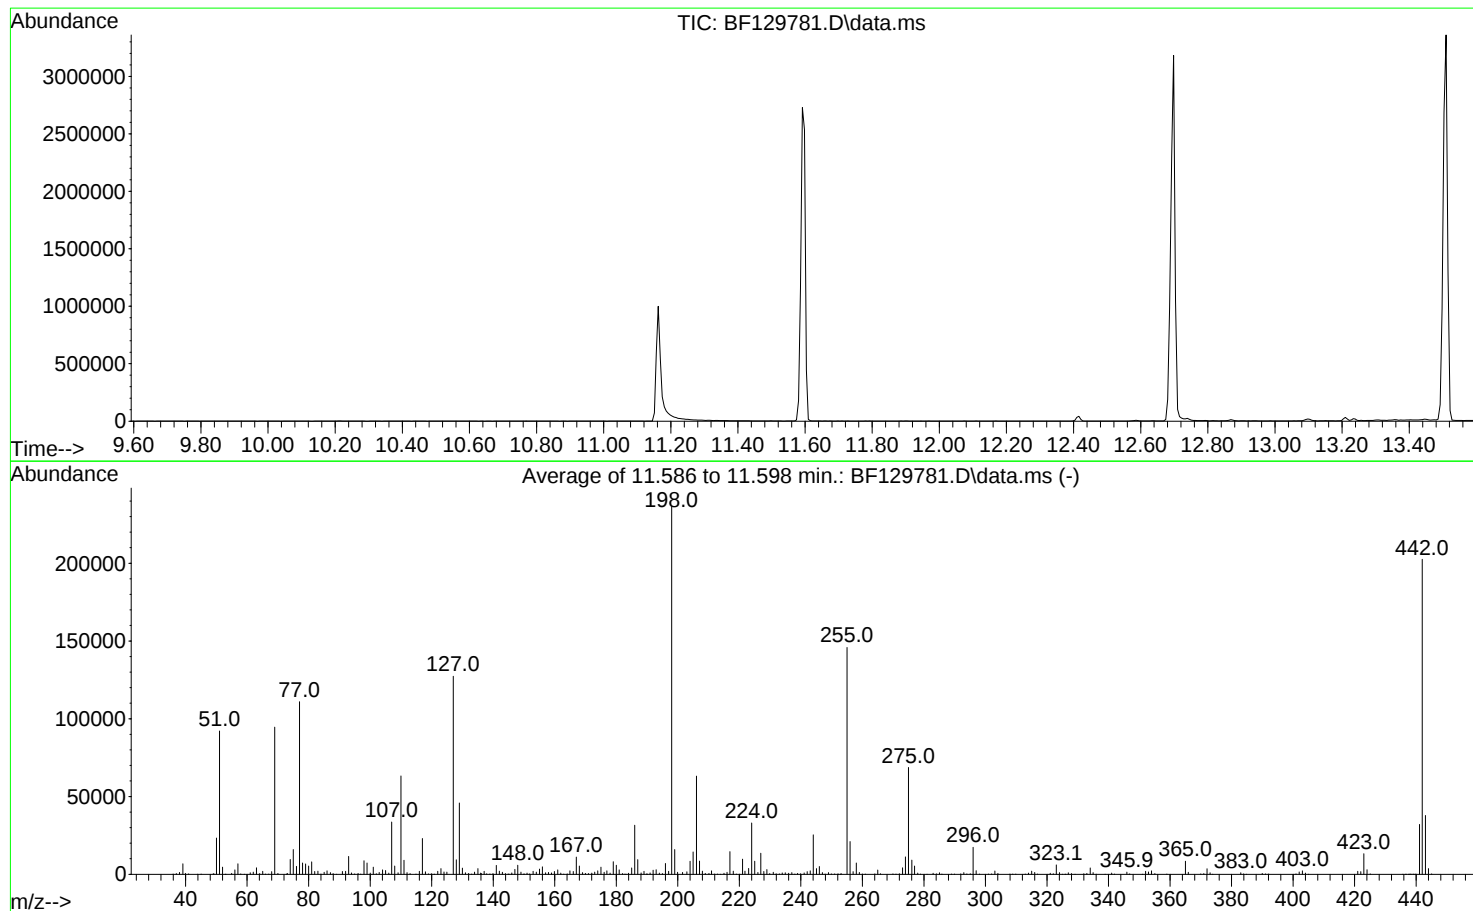




AutoFind: Scans 1581, 1582, 1583; Background Corrected with Scan 1576

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 38.9         | 92093      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1747       | PASS                |
| 69             | 198             | 0.00            | 100             | 40.0         | 94600      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 534        | PASS                |
| 127            | 198             | 10              | 80              | 53.9         | 127381     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.8          | 1927       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 236541     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 15940      | PASS                |
| 275            | 198             | 10              | 60              | 29.0         | 68693      | PASS                |
| 365            | 198             | 1               | 100             | 3.5          | 8374       | PASS                |
| 441            | 198             | 0.01            | 100             | 13.6         | 32053      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 202544     | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 37861      | PASS                |

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081522\  
Data File : BF129781.D  
Acq On    : 15 Aug 2022  15:25  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

**Instrument :**  
BNA\_F  
**ClientSampleId :**  
DFTPP

Quant Time: Aug 16 04:28:00 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 15 02:28:31 2022  
Response via : Initial Calibration

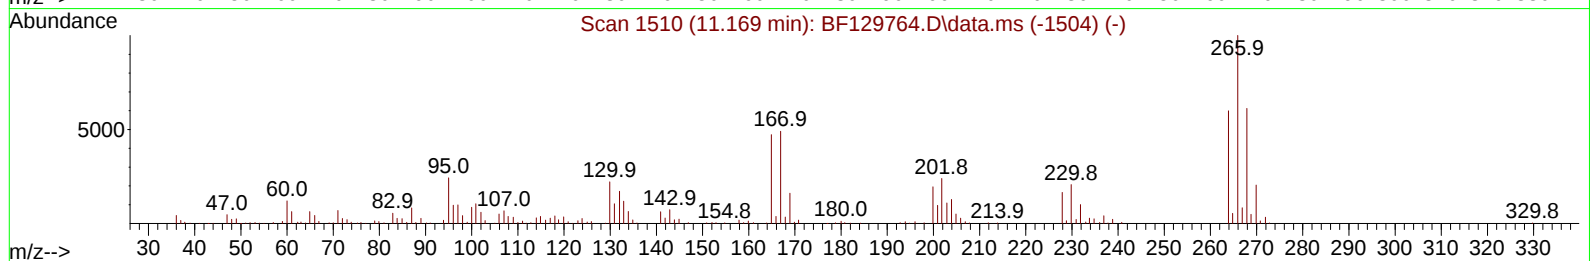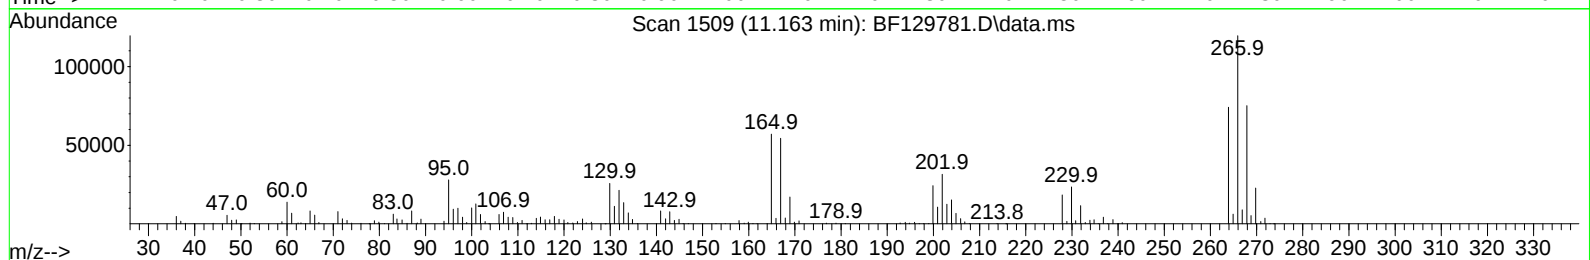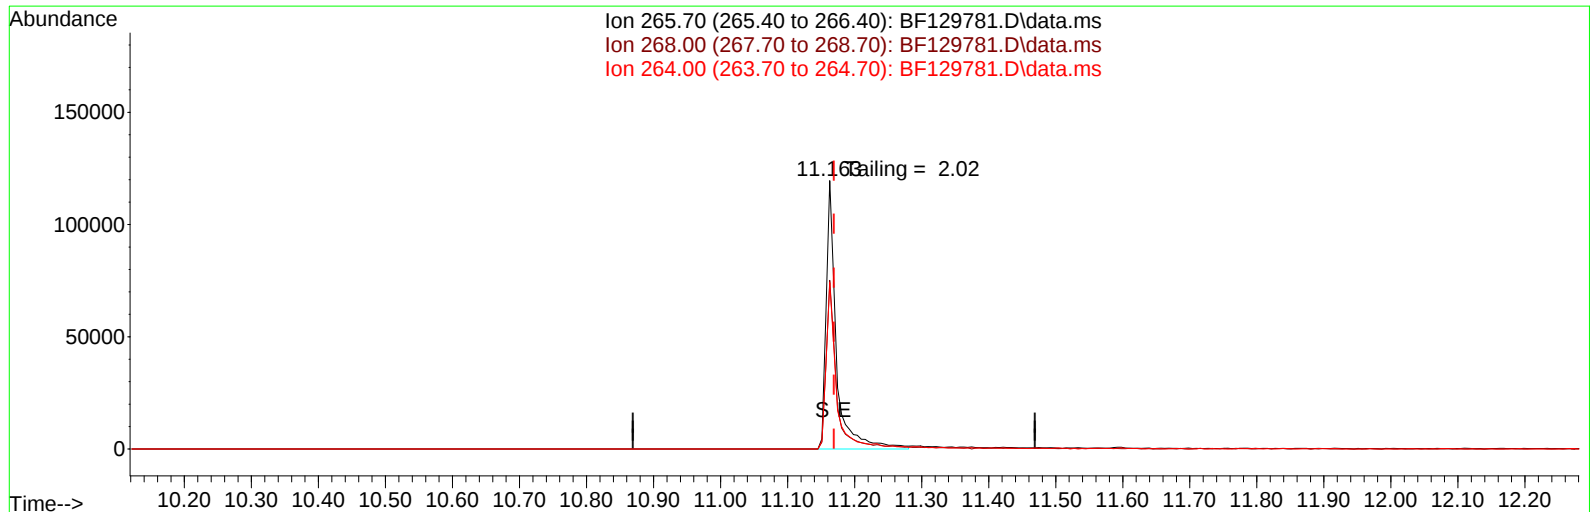

TIC: BF129781.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 32543.32 ng




**response**      **127685**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 62.87  |
| 264.00 | 59.90  | 62.03  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081522\  
Data File : BF129781.D  
Acq On : 15 Aug 2022 15:25  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 16 04:28:00 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 15 02:28:31 2022  
Response via : Initial Calibration

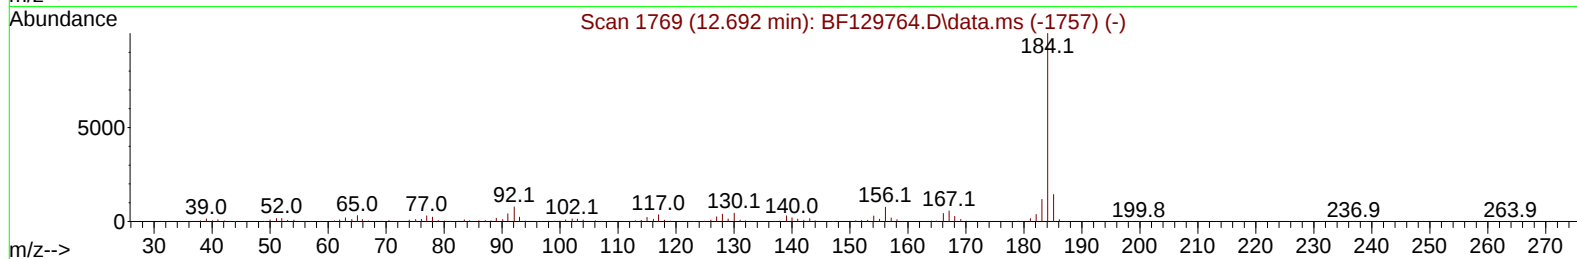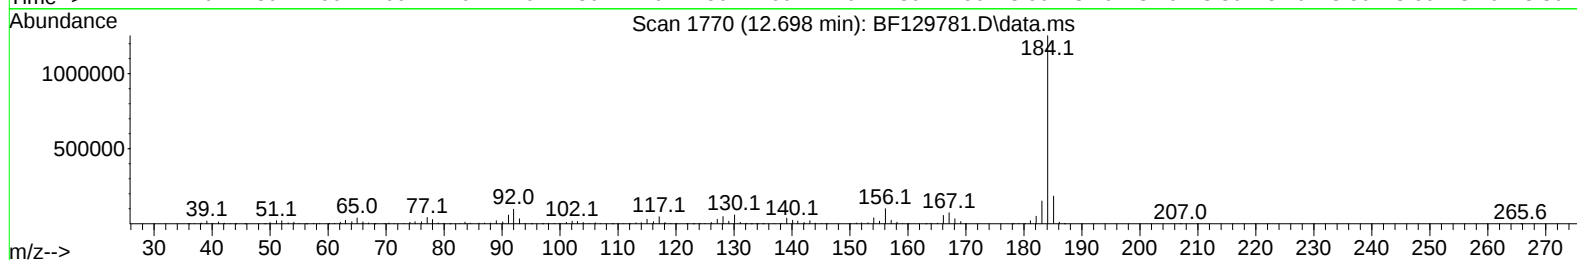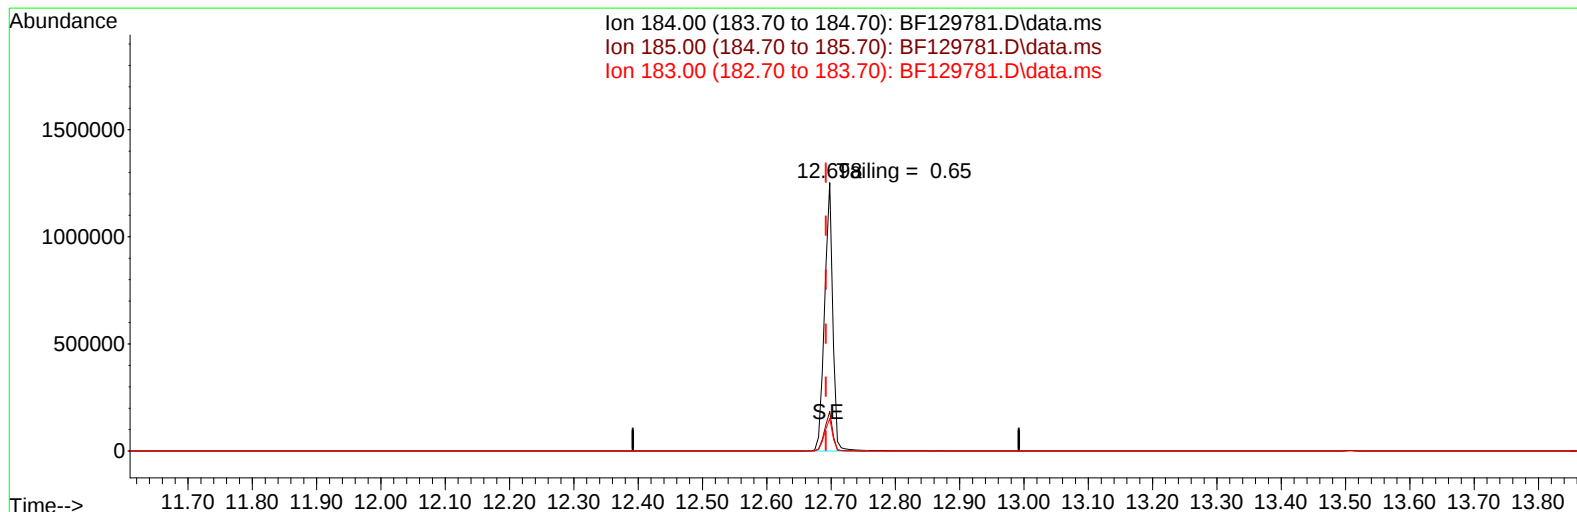

TIC: BF129781.D\data.ms

**(77) Benzidine**

**12.698min (+ 0.006) 0.00 ng**

**response 1116885**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 14.76  |
| 183.00 | 11.80  | 12.10  |
| 0.00   | 0.00   | 0.00   |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/15/2022     | BNA_F            | <u>BF129781.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 590537           | 13.51              |
| DDD           | 8718             | 13.21              |
| DDE           | 2051             | 12.869             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10769         | 601306           | 1.79               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP