
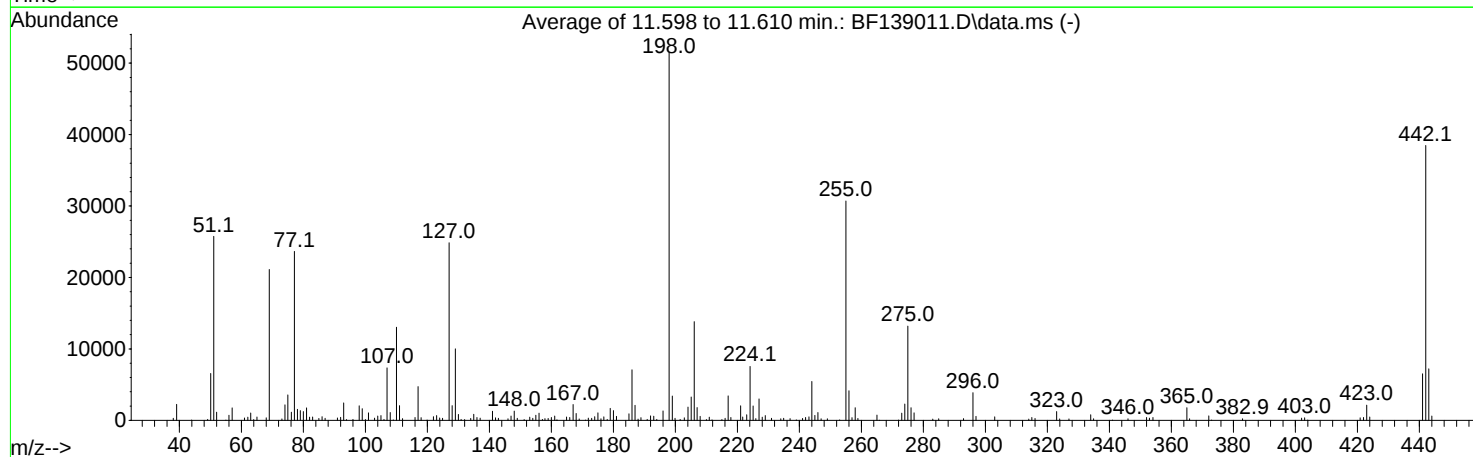


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081524\
Data File : BF139011.D
Acq On : 15 Aug 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

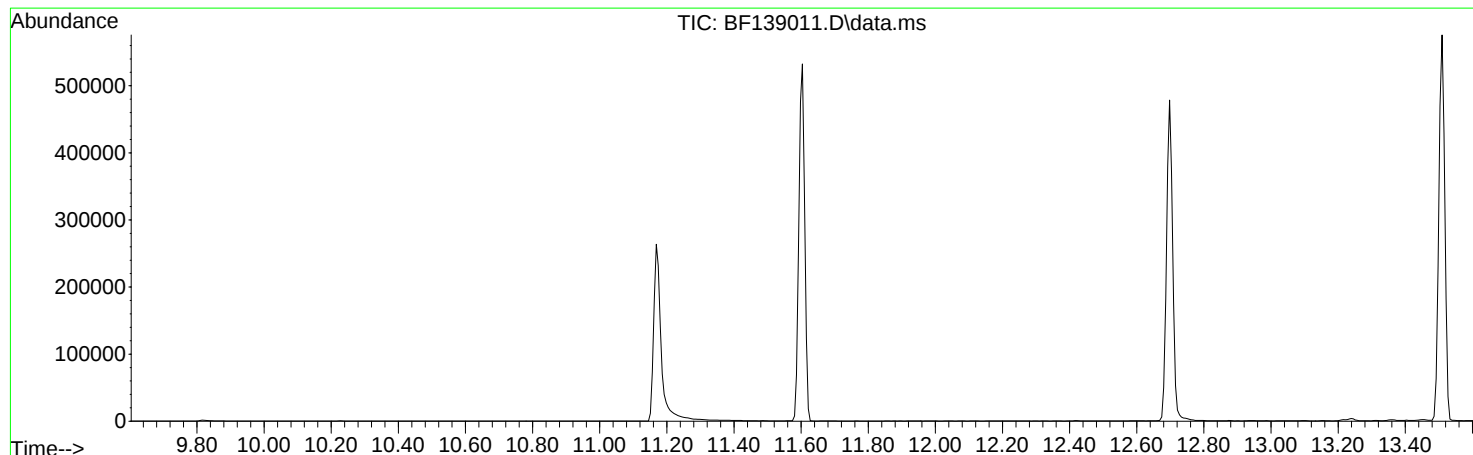




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.0	25752	PASS
68	69	0.00	2	1.7	364	PASS
69	198	0.00	100	41.0	21122	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	24861	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51488	PASS
199	198	5	9	6.6	3404	PASS
275	198	10	60	25.6	13194	PASS
365	198	1	100	3.5	1781	PASS
441	198	0.01	100	12.7	6527	PASS
442	442	50	100	100.0	38483	PASS
443	442	15	24	18.7	7206	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081524\
Data File : BF139011.D
Acq On : 15 Aug 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 12:05:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

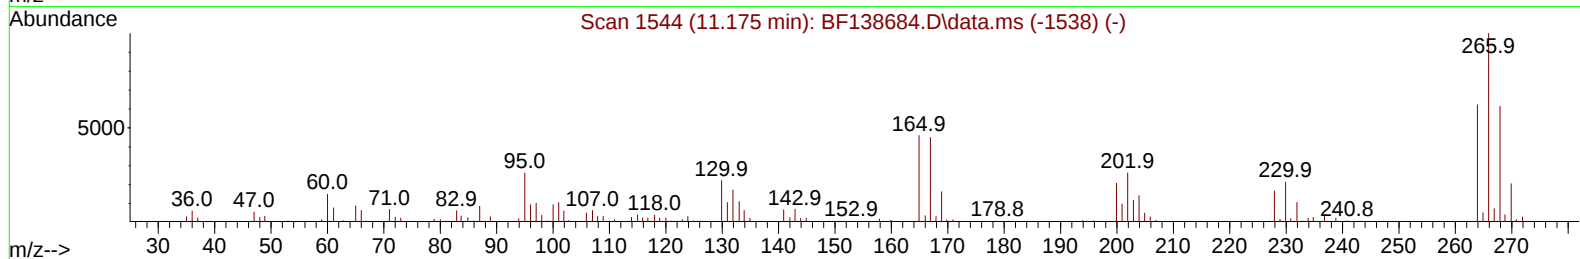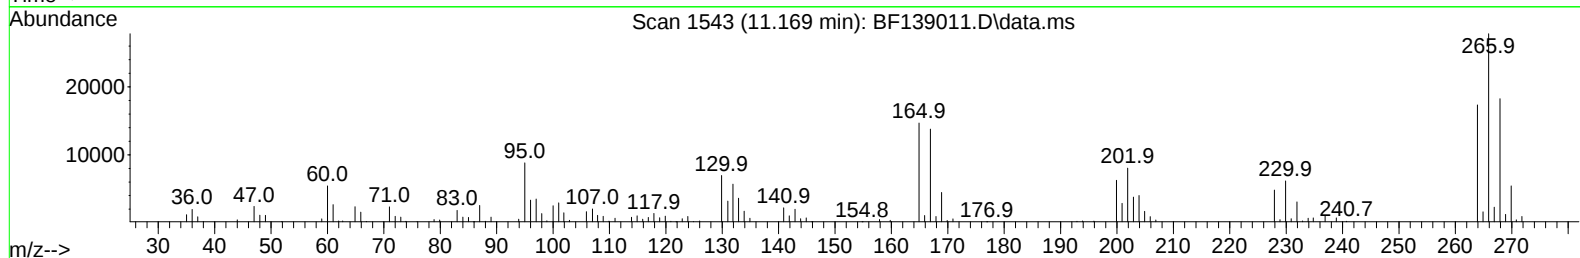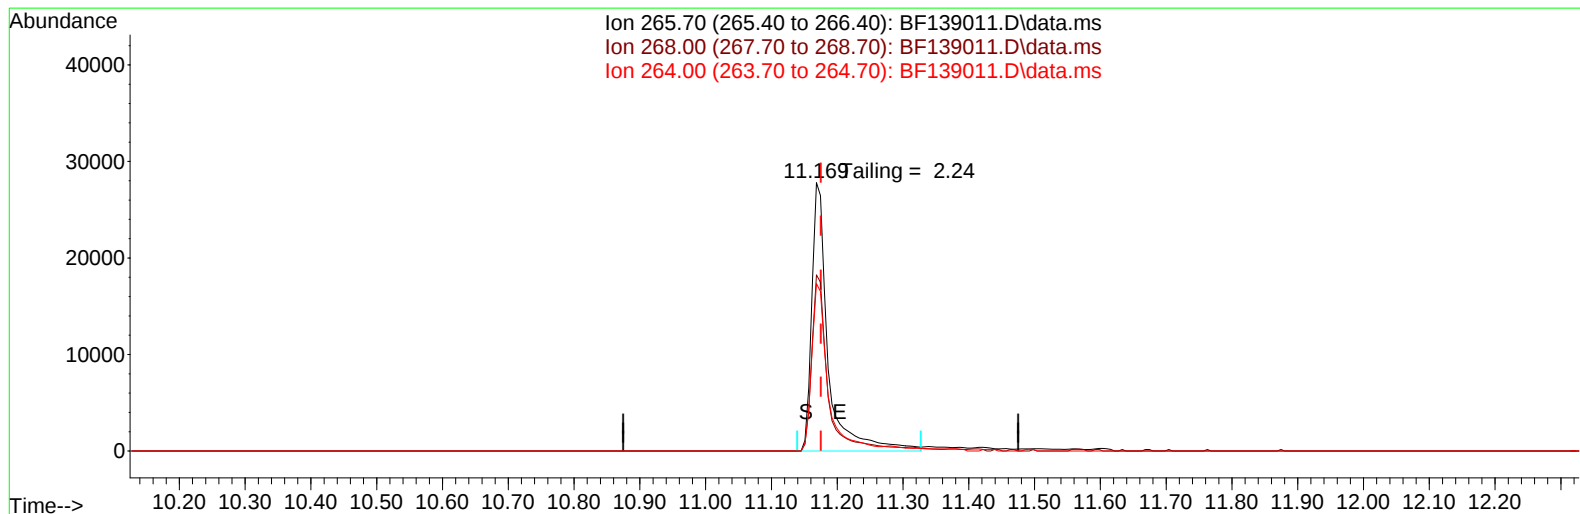

TIC: BF139011.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 47919.90 ng m




response 48533

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	65.65
264.00	62.20	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081524\
Data File : BF139011.D
Acq On : 15 Aug 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 12:05:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

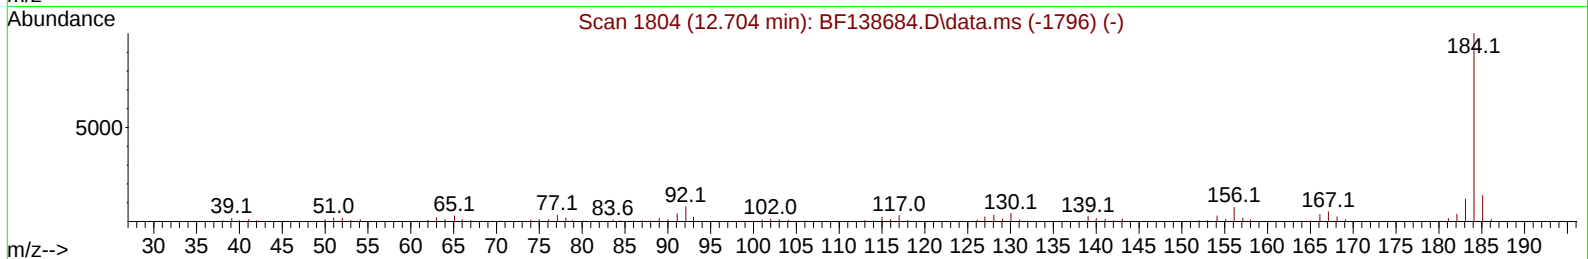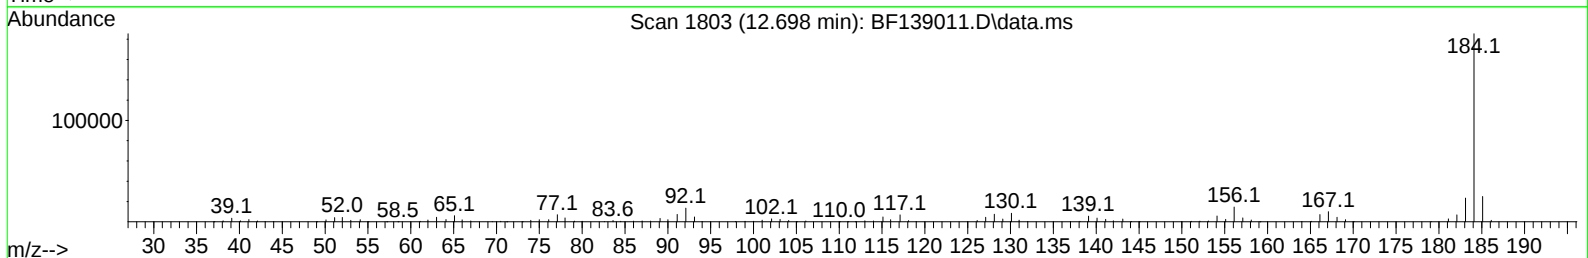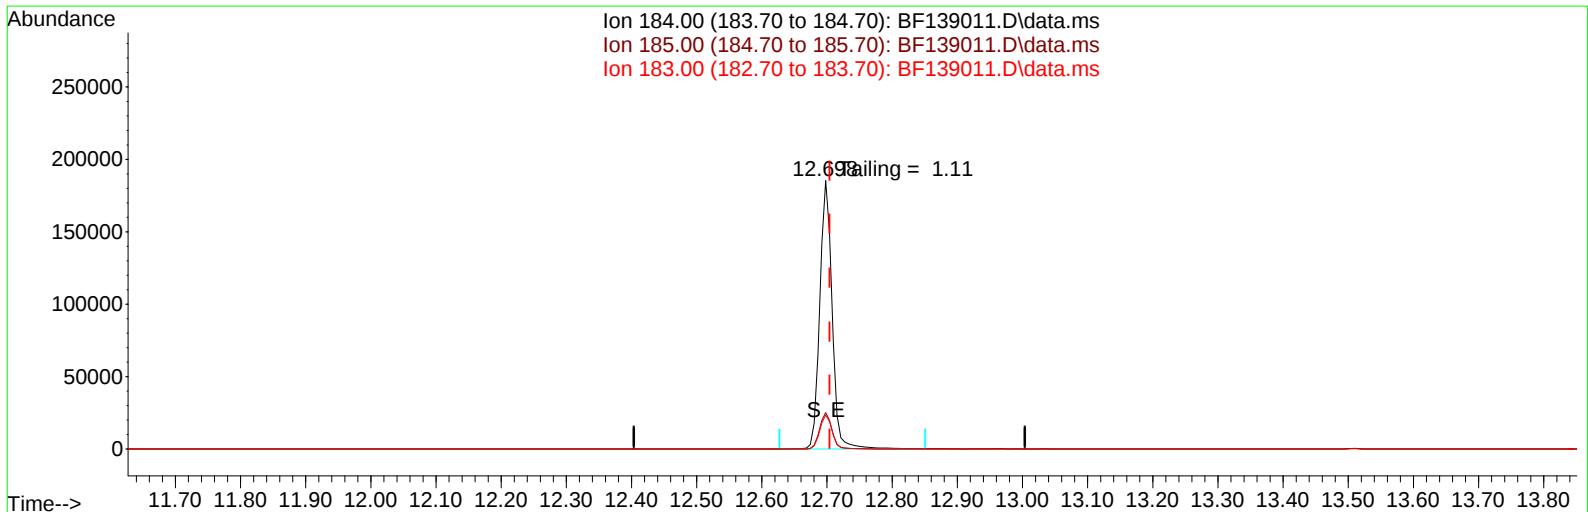

TIC: BF139011.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 245453

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.56
183.00	12.00	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2024	BNA_F	<u>BF139011.D</u>
Compound Name	Response	Retention Time
DDT	134295	13.51
DDD	2233	13.239
DDE	264	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2497	136792	1.83

Instrument :
BNA_F
ClientSampleId :
DFTPP