
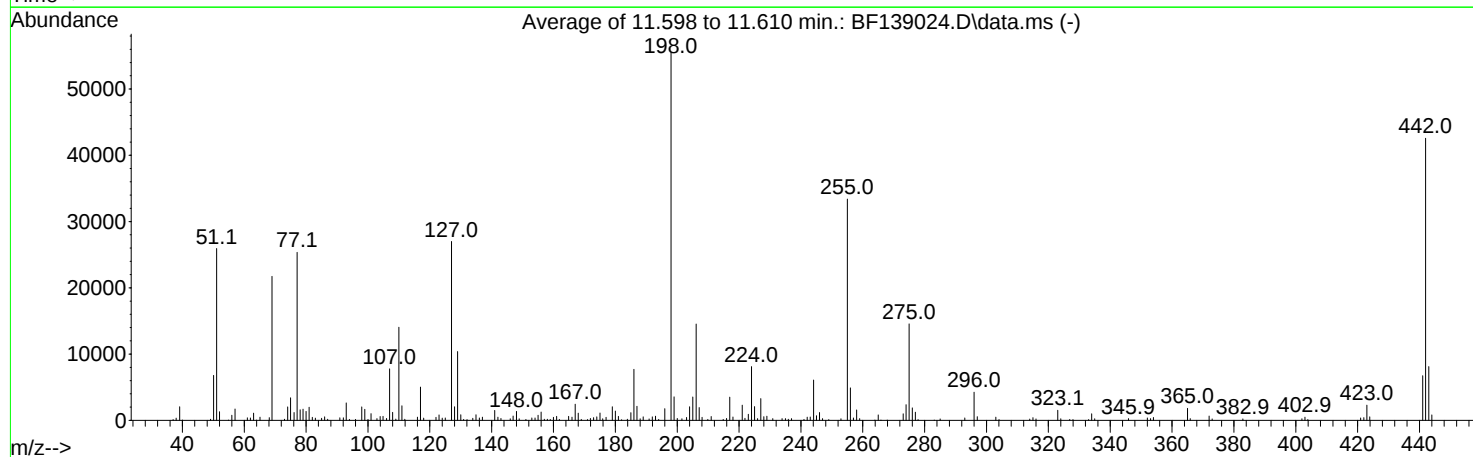


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081524\
Data File : BF139024.D
Acq On : 15 Aug 2024 16:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

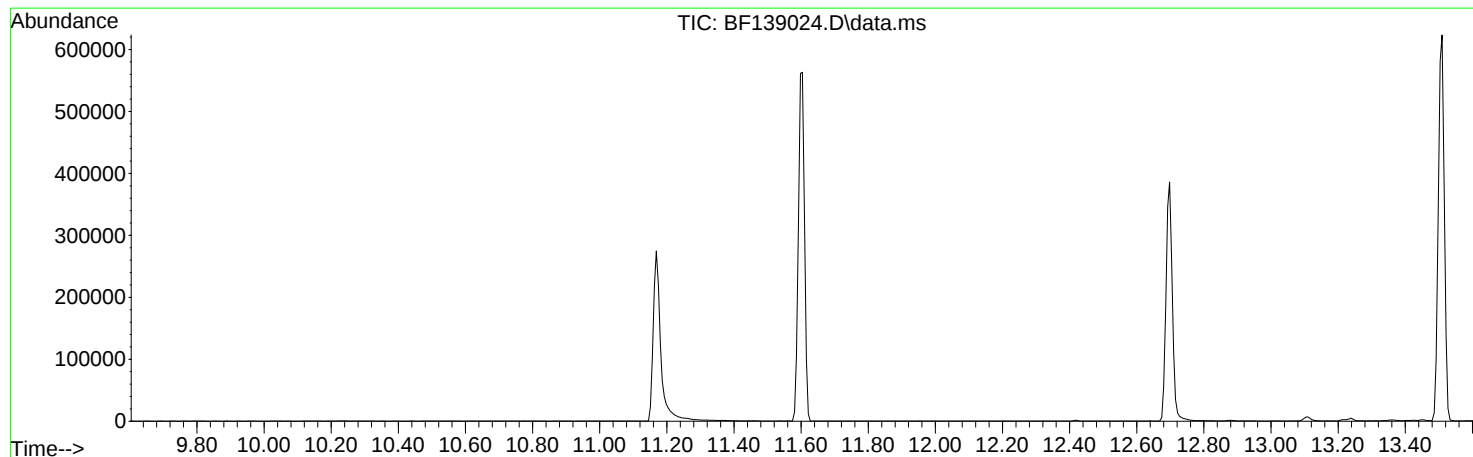




AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	25940	PASS
68	69	0.00	2	1.9	410	PASS
69	198	0.00	100	39.1	21727	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	27000	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55512	PASS
199	198	5	9	6.4	3546	PASS
275	198	10	60	26.2	14571	PASS
365	198	1	100	3.3	1818	PASS
441	198	0.01	100	12.1	6734	PASS
442	442	50	100	100.0	42581	PASS
443	442	15	24	19.1	8124	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081524\
Data File : BF139024.D
Acq On : 15 Aug 2024 16:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 17:03:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

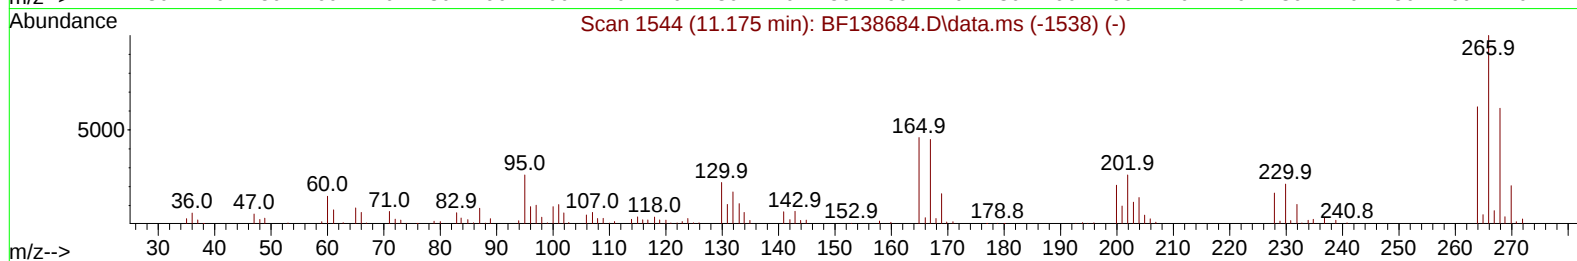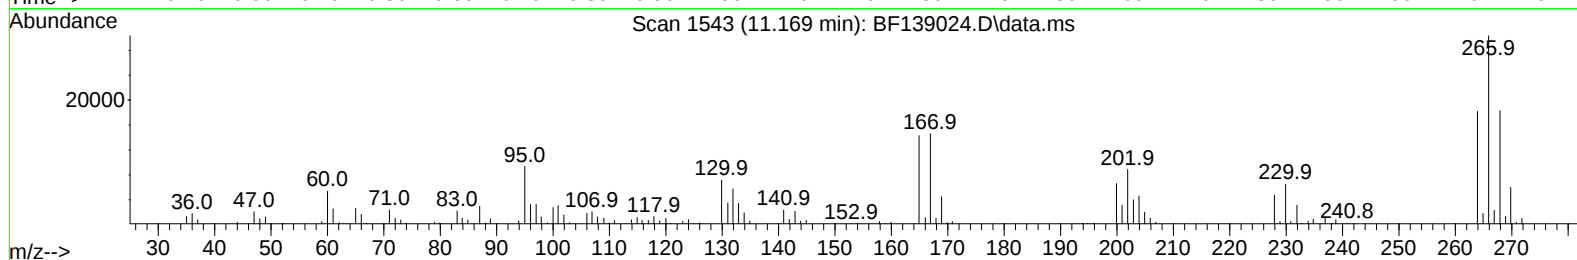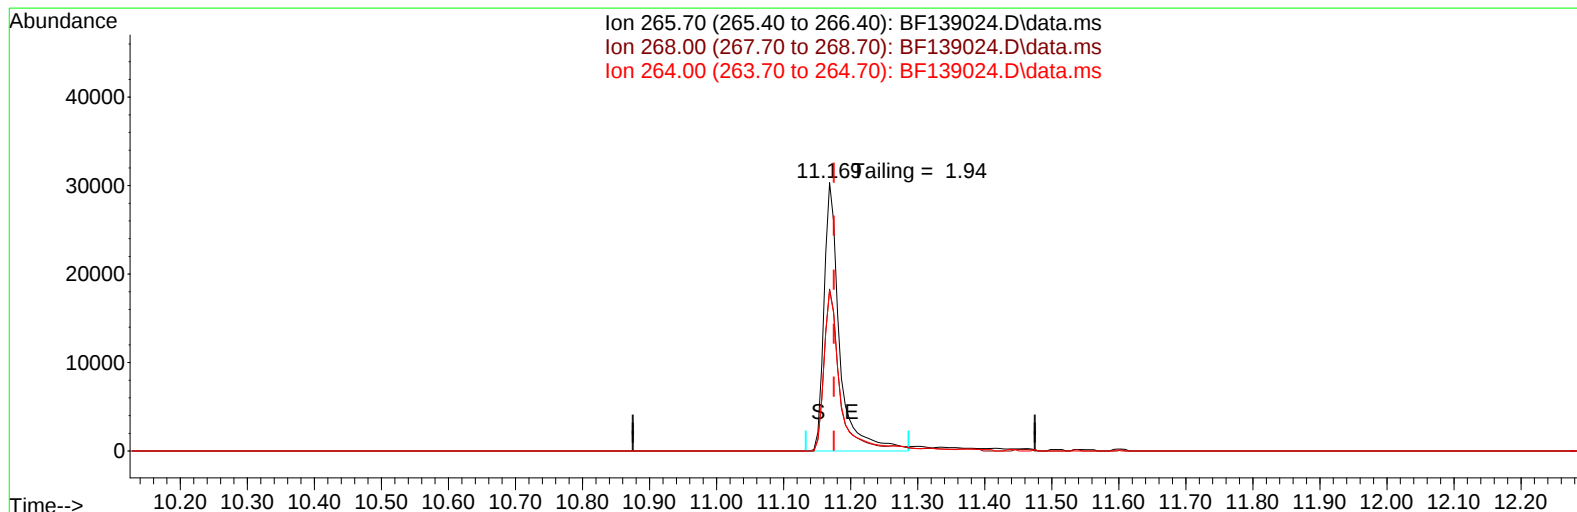

TIC: BF139024.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 39319.06 ng




response 49530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	60.36
264.00	62.20	59.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081524\
Data File : BF139024.D
Acq On : 15 Aug 2024 16:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 17:03:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

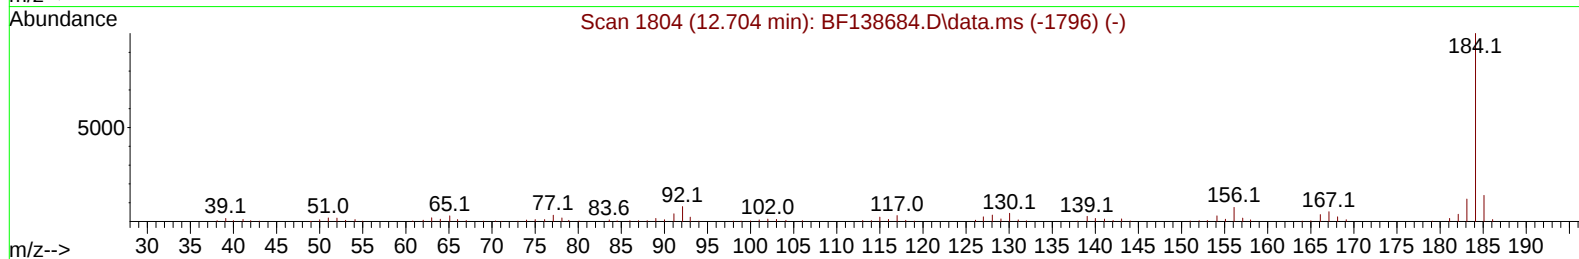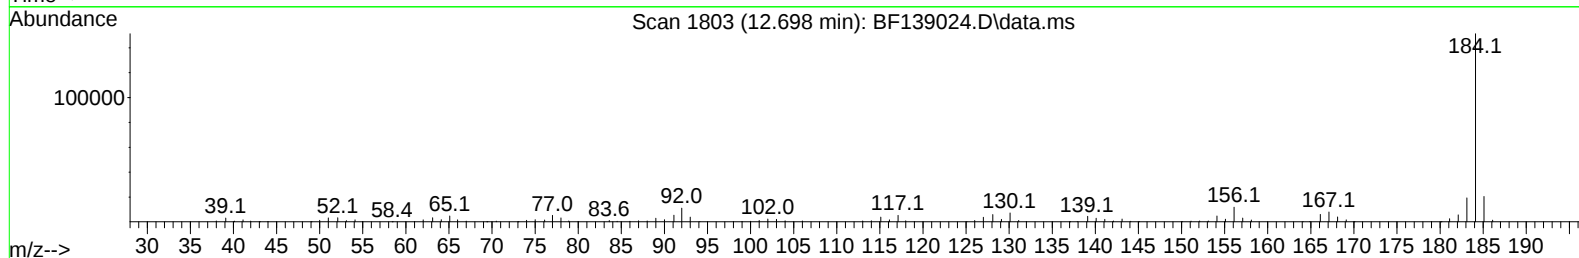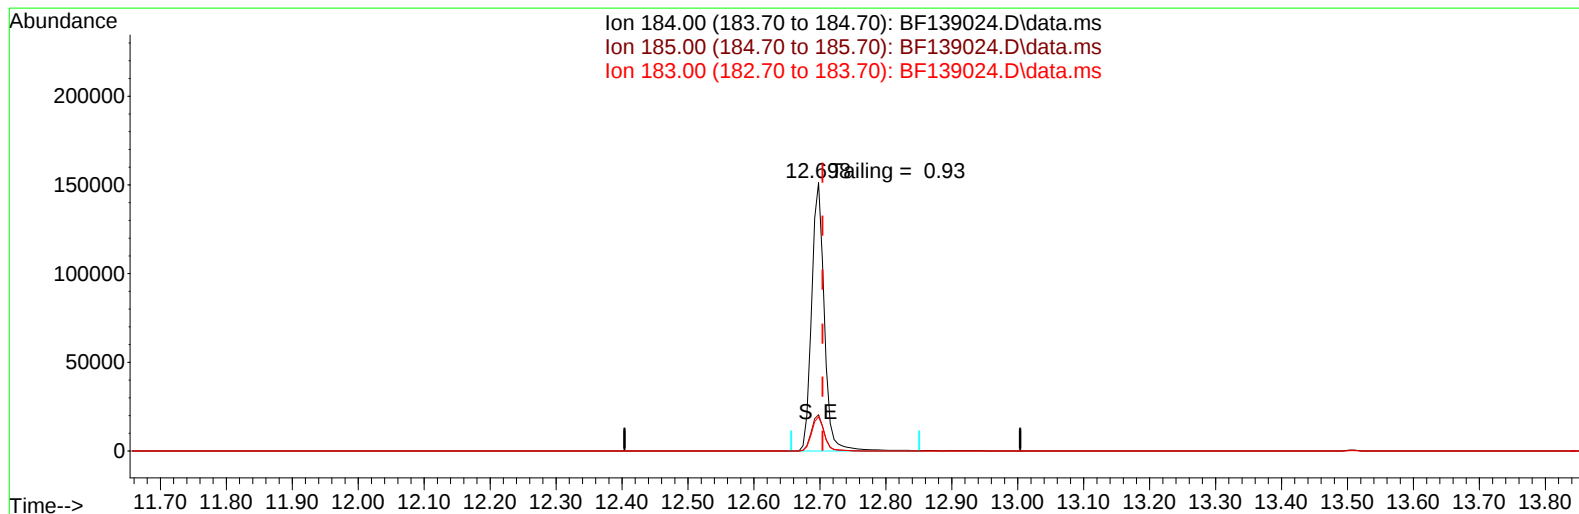

TIC: BF139024.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 202594

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.54
183.00	12.00	12.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/15/2024	BNA_F	<u>BF139024.D</u>
Compound Name	Response	Retention Time
DDT	148050	13.51
DDD	2408	13.239
DDE	515	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2923	150973	1.94

Instrument :
BNA_F
ClientSampleId :
DFTPP