
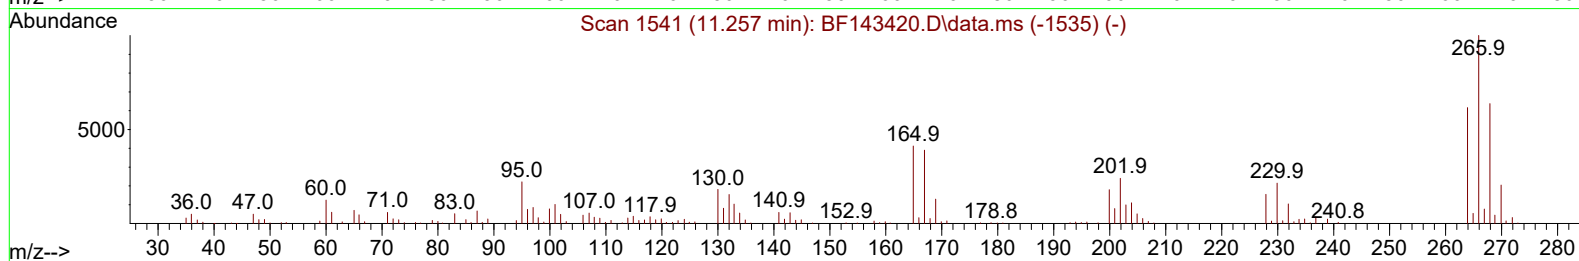
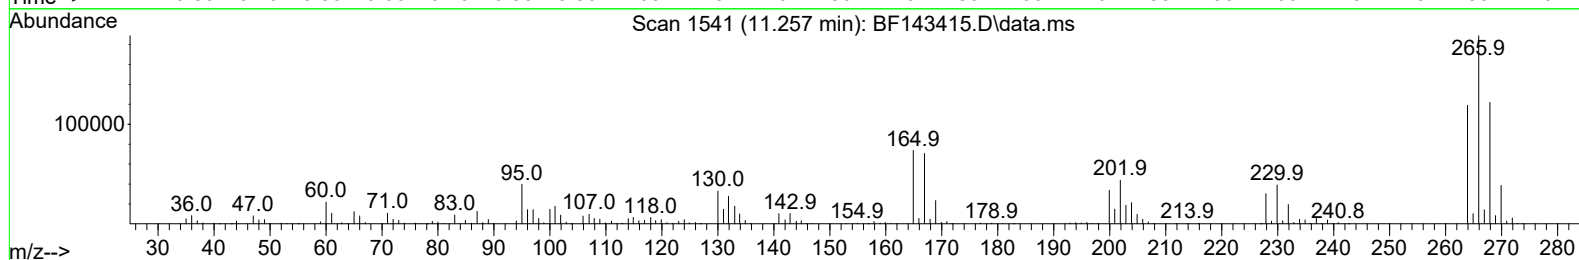


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081525\
Data File : BF143415.D
Acq On : 15 Aug 2025 13:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 19:00:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 15 18:57:34 2025
Response via : Initial Calibration

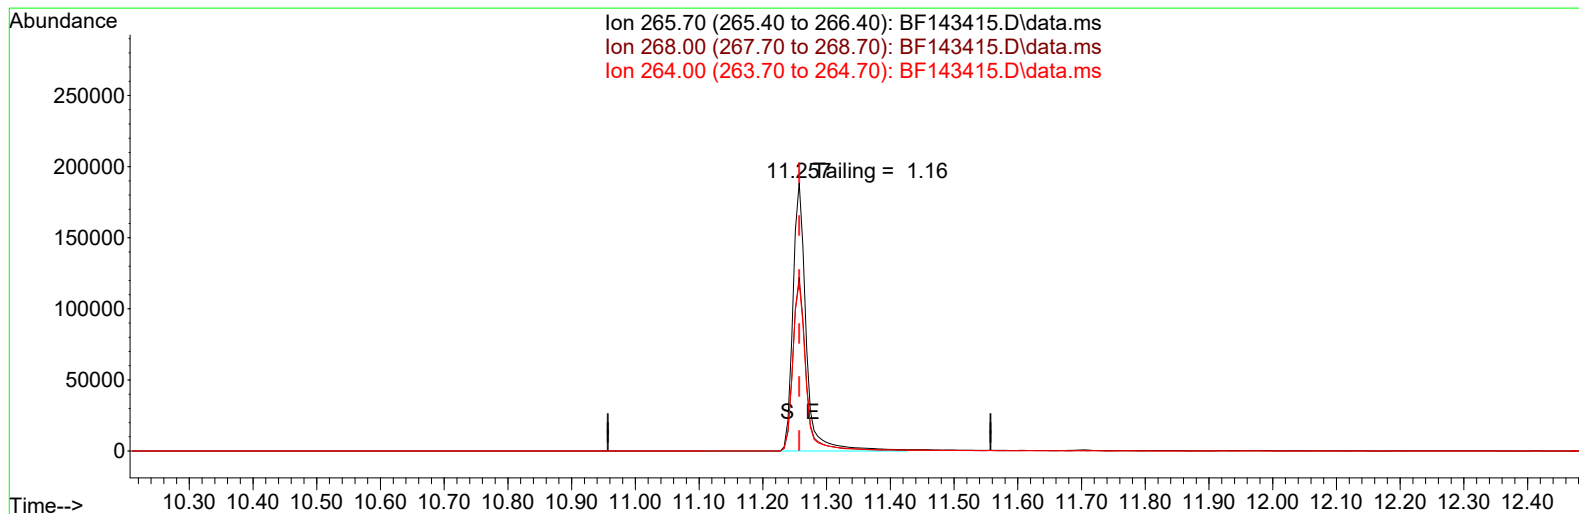

TIC: BF143415.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 361177.43 ng

response 277163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.59
264.00	61.60	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081525\
Data File : BF143415.D
Acq On : 15 Aug 2025 13:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 15 19:00:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 15 18:57:34 2025
Response via : Initial Calibration

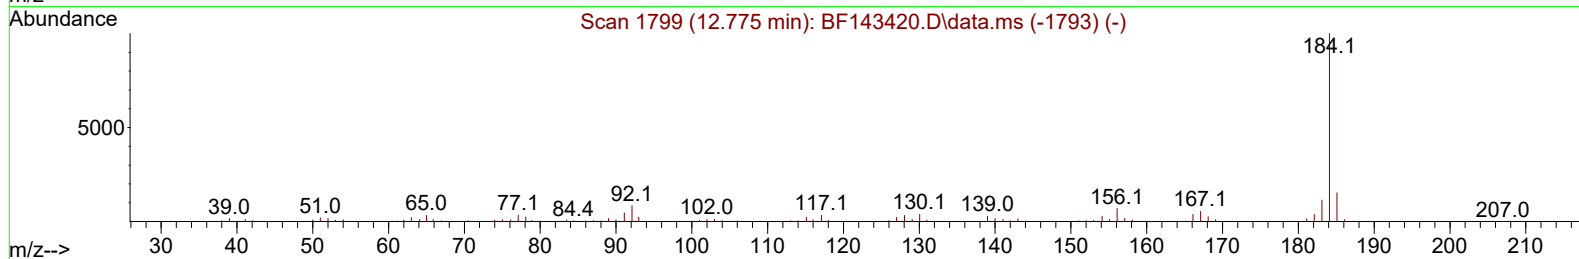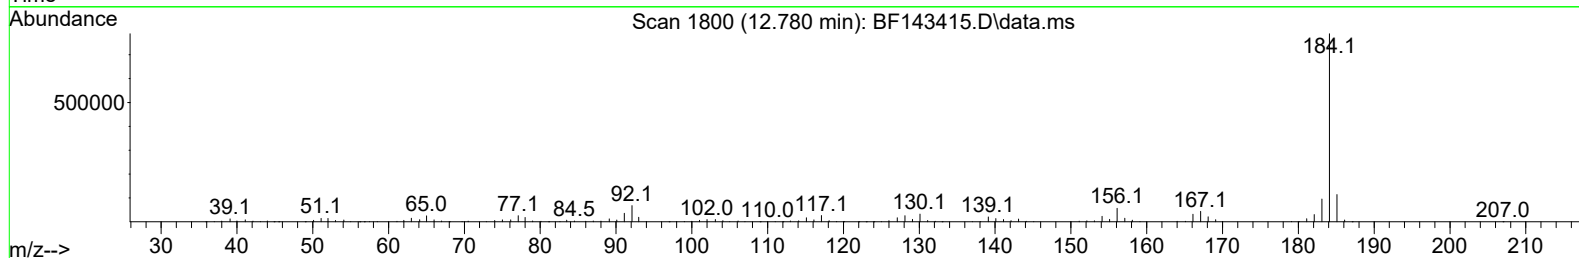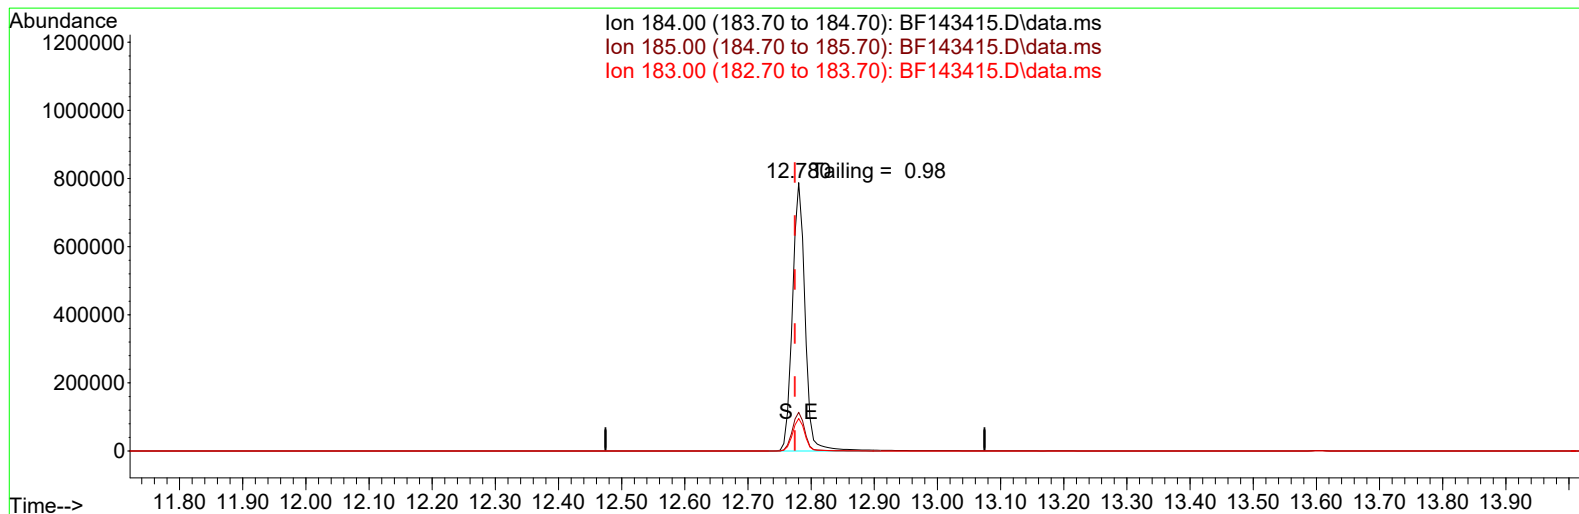

TIC: BF143415.D\data.ms

(77) Benzidine**12.780min (+ 0.006) 168452.64 ng****response 1096798**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.46
183.00	11.50	12.10
0.00	0.00	0.00