
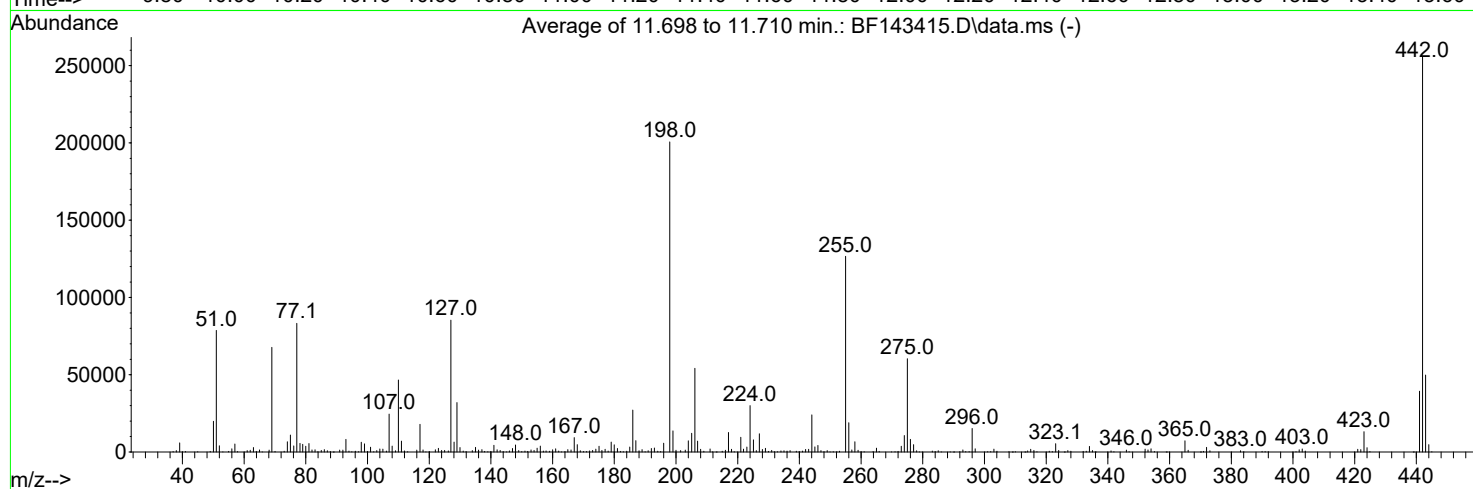


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081525\
Data File : BF143415.D
Acq On : 15 Aug 2025 13:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 18 04:40:19 2025

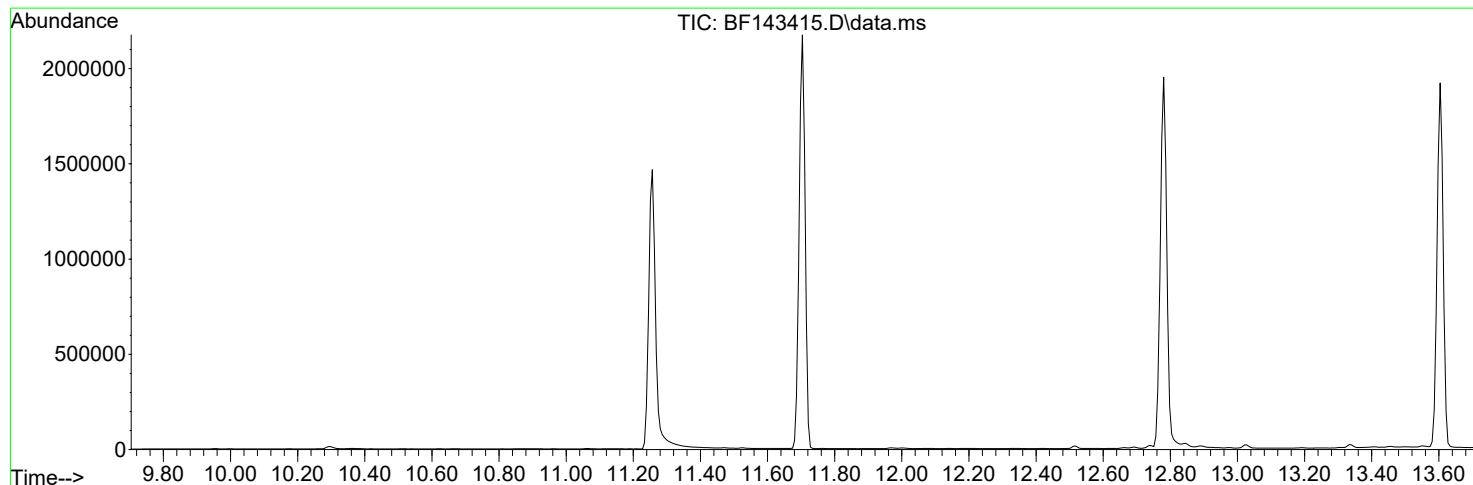

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	1264	PASS
69	69	100	100	100.0	67720	PASS
70	69	0.00	2	0.6	406	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	200640	PASS
199	198	5	9	6.8	13673	PASS
365	198	1	100	3.6	7304	PASS
441	443	0.01	150	79.0	39347	PASS
442	442	100	100	100.0	255488	PASS
443	442	15	24	19.5	49795	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/15/2025	BNA_F	BF143415.D
Compound Name	Response	Retention Time
DDT	478181	13.604
DDD	9101	13.339
DDE		13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9101	487282	1.87

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081525\
Data File : BF143415.D
Acq On : 15 Aug 2025 13:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 19:00:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 15 18:57:34 2025
Response via : Initial Calibration

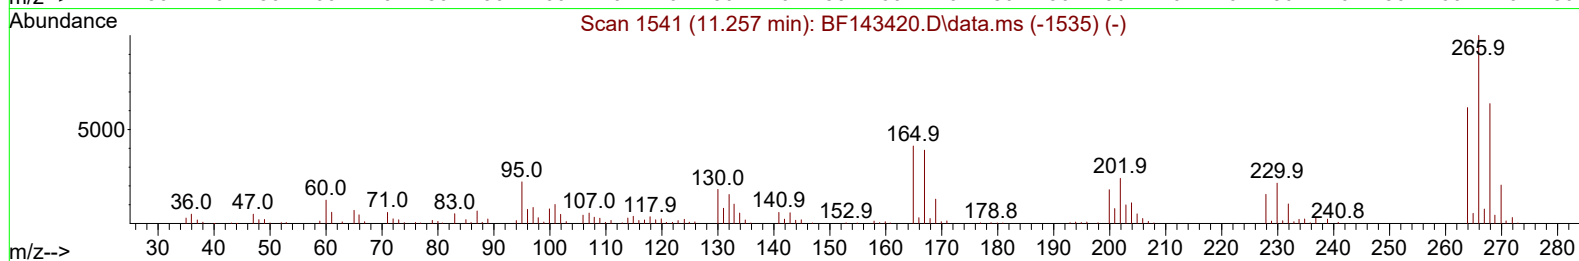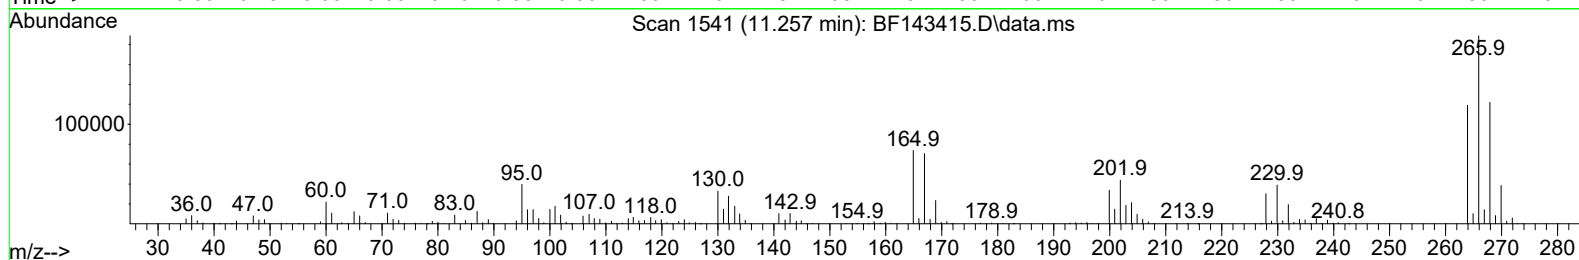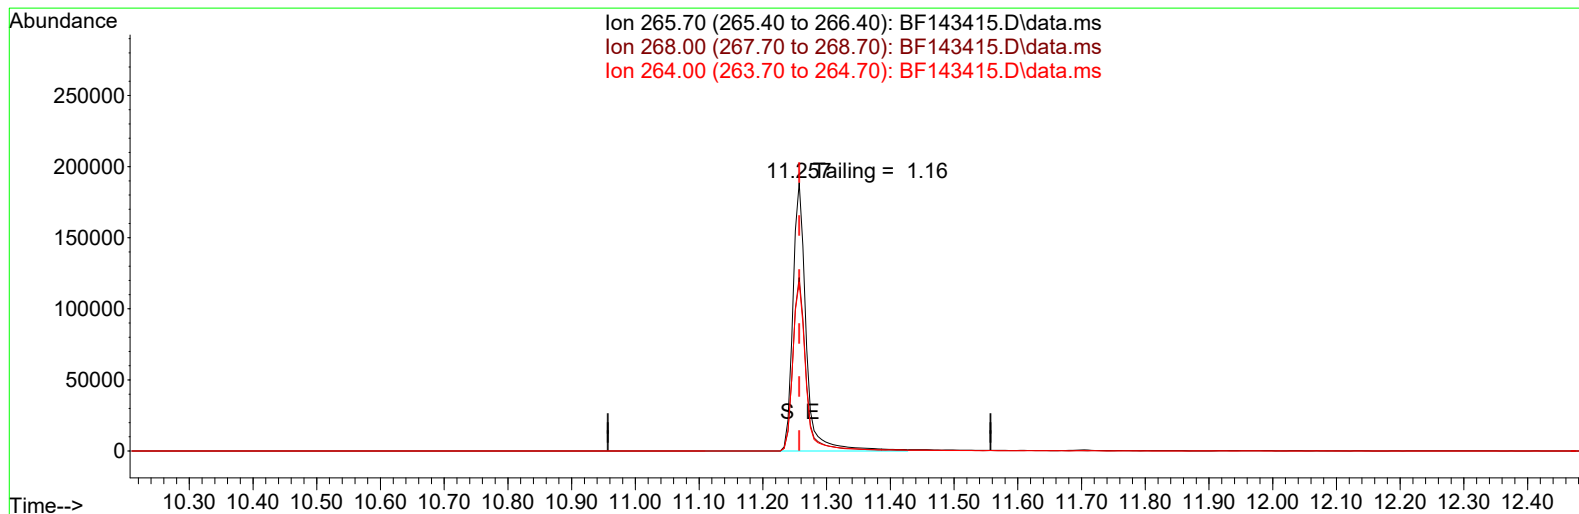

TIC: BF143415.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 361177.43 ng




response 277163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.59
264.00	61.60	62.99
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081525\  
Data File : BF143415.D  
Acq On    : 15 Aug 2025   13:59  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 15 19:00:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 15 18:57:34 2025
Response via : Initial Calibration

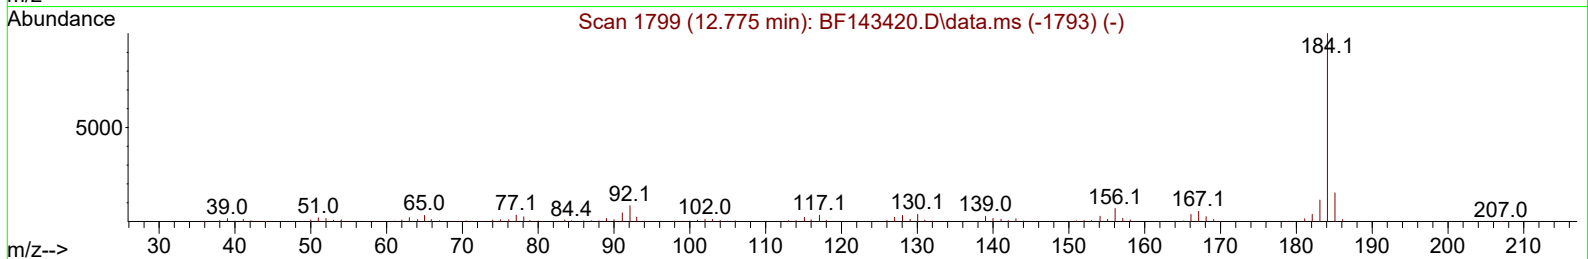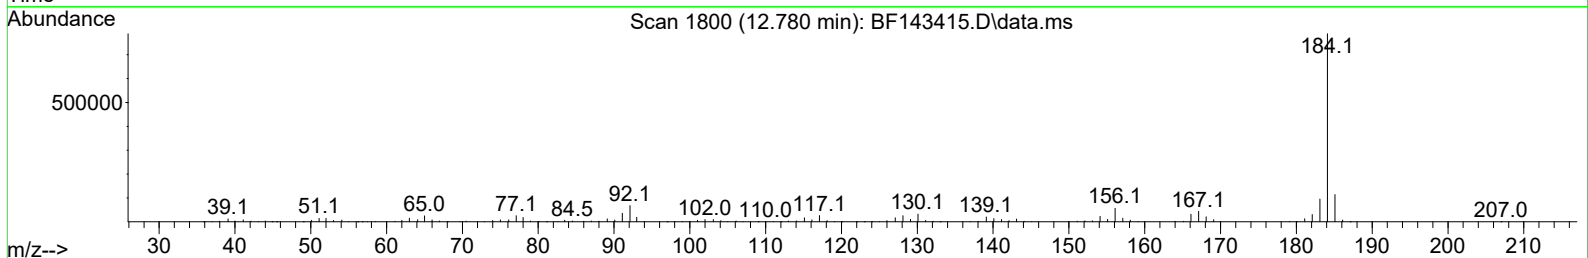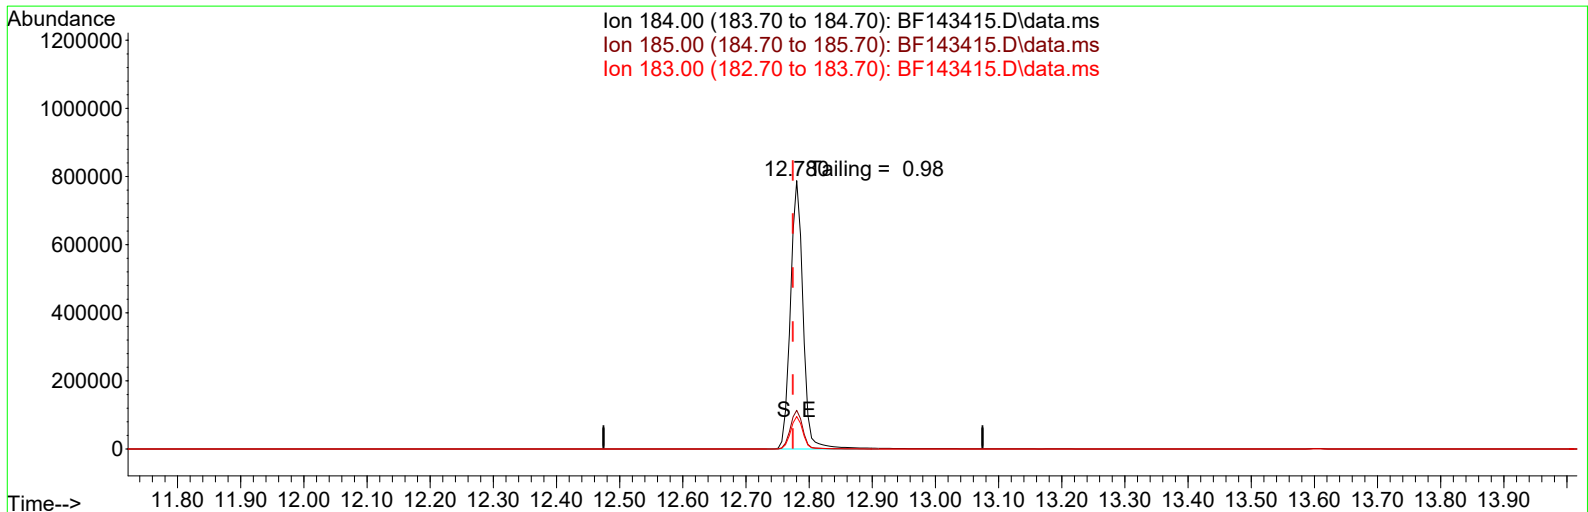

TIC: BF143415.D\data.ms

(77) Benzidine

12.780min (+ 0.006) 168452.64 ng

response **1096798**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.46
183.00	11.50	12.10
0.00	0.00	0.00