


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081616\
 Data File : BF089725.D
 Acq On : 16 Aug 2016 15:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 16 19:45:04 2016

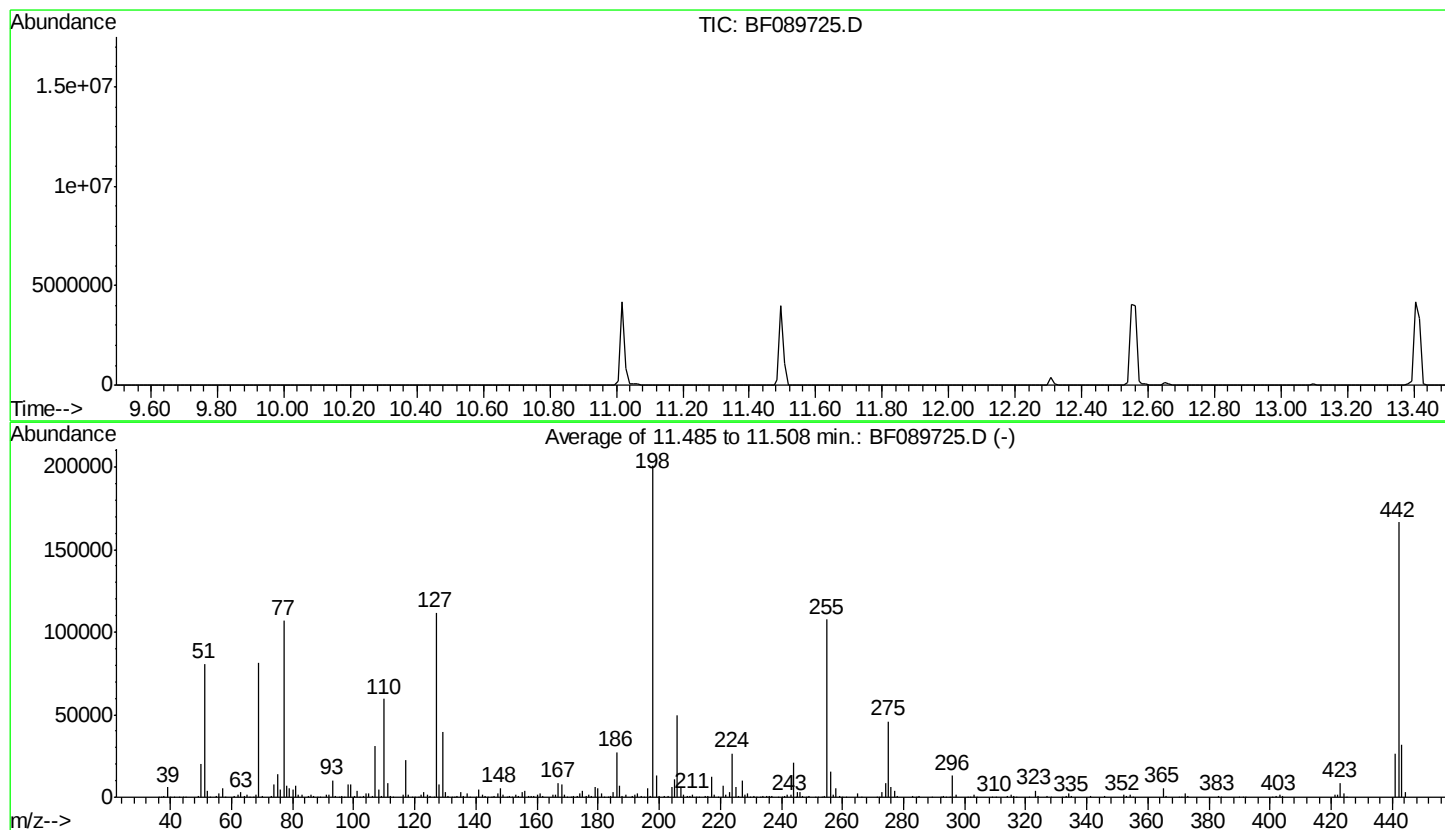

AutoFind: Scans 866, 867, 868; Background Corrected with Scan 863

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	80996	PASS
68	69	0.00	2	1.6	1317	PASS
69	198	0.00	100	40.4	81125	PASS
70	69	0.00	2	0.7	606	PASS
127	198	10	80	55.6	111682	PASS
197	198	0.00	2	0.5	957	PASS
198	198	100	100	100.0	200864	PASS
199	198	5	9	6.7	13549	PASS
275	198	10	60	22.8	45877	PASS
365	198	1	100	2.8	5565	PASS
441	442	0.01	24	16.0	26683	PASS
442	198	50	100	83.0	166692	PASS
443	442	15	24	19.3	32098	PASS