


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF081616\
 Data File : BF089734.D
 Acq On : 17 Aug 2016 00:57
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 16 19:45:04 2016

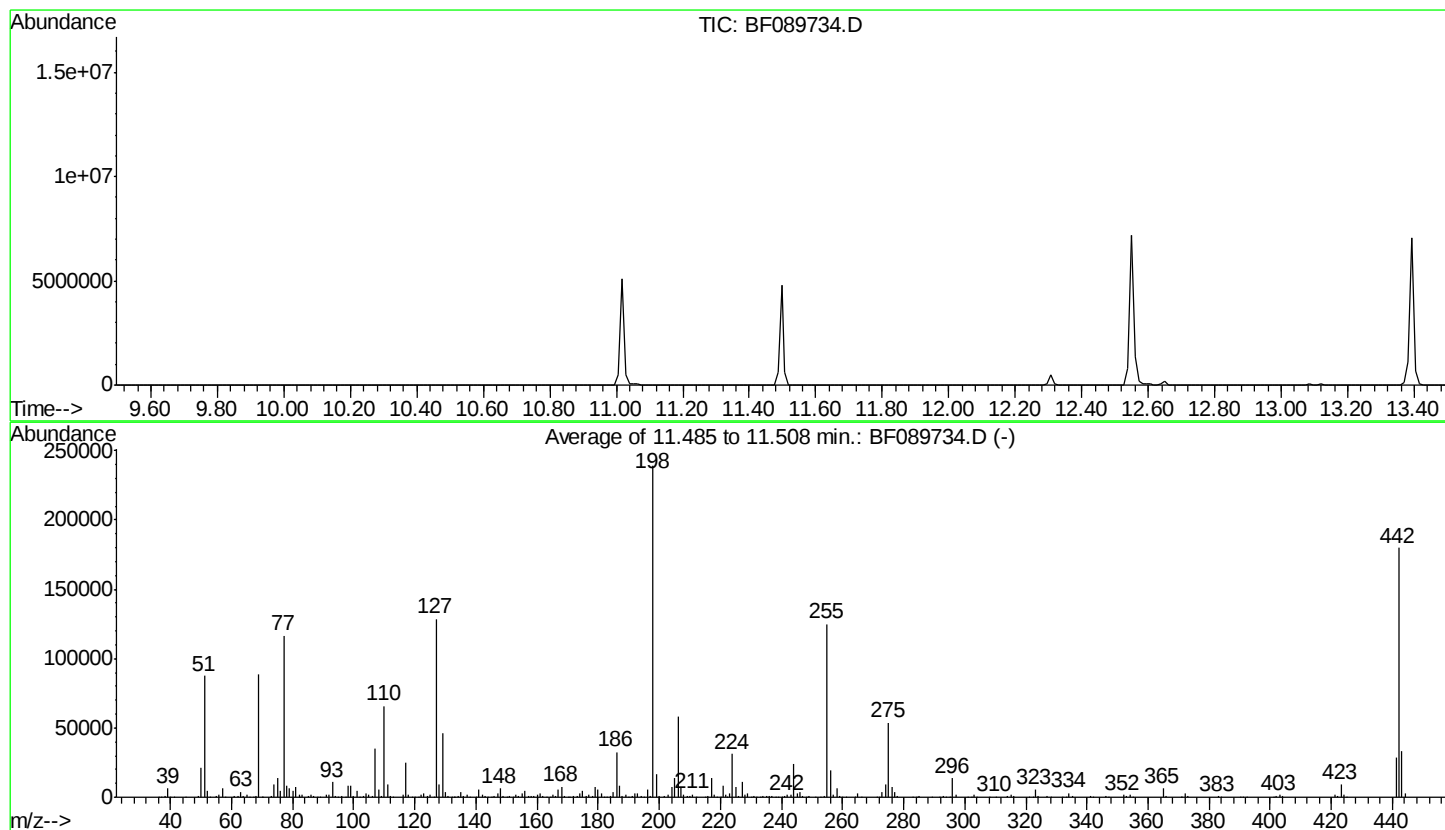

AutoFind: Scans 866, 867, 868; Background Corrected with Scan 862

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	87384	PASS
68	69	0.00	2	1.5	1302	PASS
69	198	0.00	100	37.2	88891	PASS
70	69	0.00	2	0.5	429	PASS
127	198	10	80	53.8	128813	PASS
197	198	0.00	2	0.4	929	PASS
198	198	100	100	100.0	239232	PASS
199	198	5	9	6.8	16227	PASS
275	198	10	60	22.5	53792	PASS
365	198	1	100	2.6	6217	PASS
441	442	0.01	24	16.1	29009	PASS
442	198	50	100	75.2	179965	PASS
443	442	15	24	18.7	33650	PASS