


Data Path : Z:\HPCHEM1\BNA F\Data\BF081617\
 Data File : BF097733.D
 Acq On : 16 Aug 2017 12:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

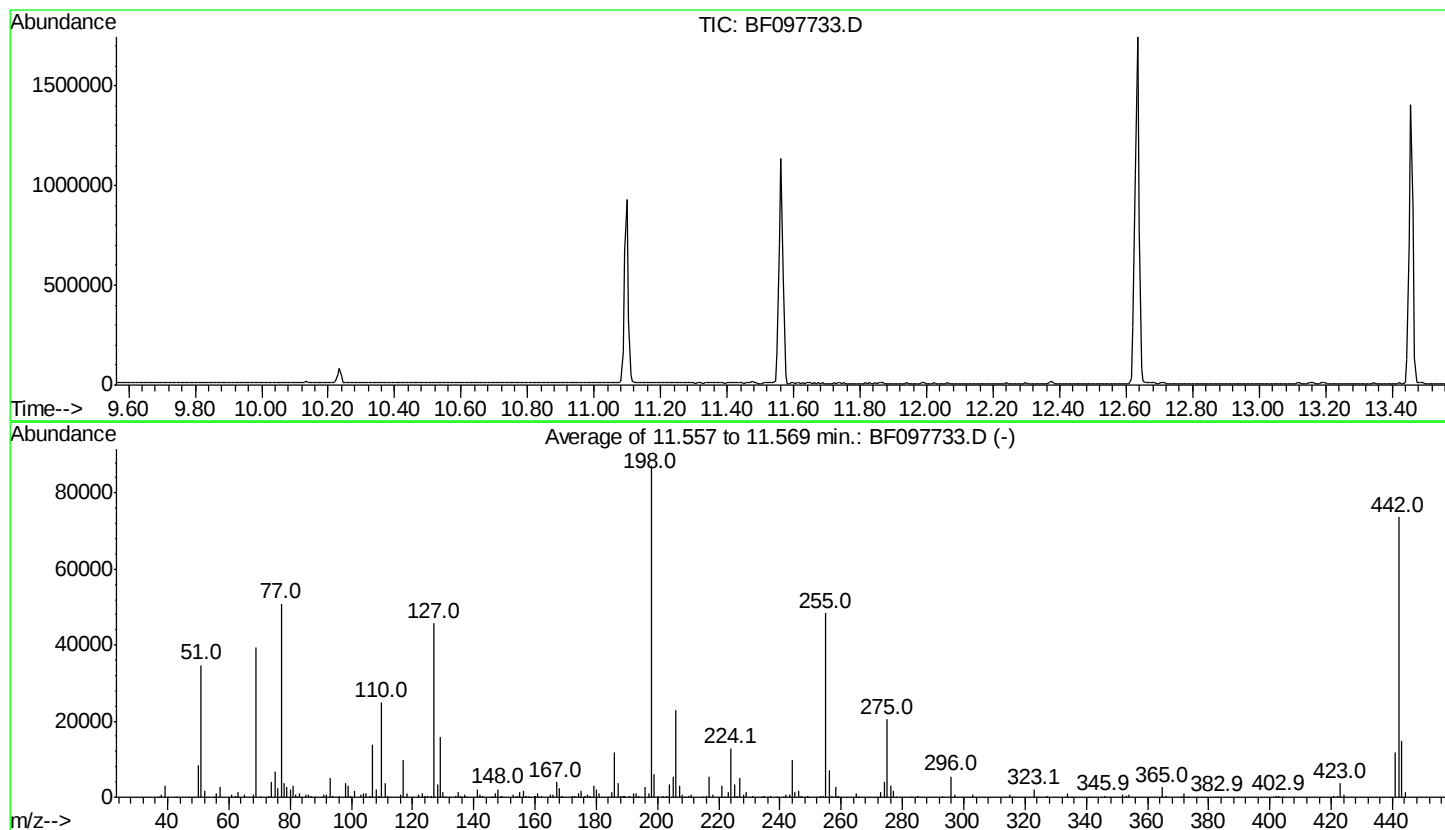

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	34770	PASS
68	69	0.00	2	1.7	682	PASS
69	198	0.00	100	45.1	39306	PASS
70	69	0.00	2	0.4	156	PASS
127	198	10	80	52.4	45717	PASS
197	198	0.00	2	1.0	852	PASS
198	198	100	100	100.0	87173	PASS
199	198	5	9	6.8	5919	PASS
275	198	10	60	23.4	20440	PASS
365	198	1	100	2.9	2550	PASS
441	442	0.01	24	15.9	11693	PASS
442	198	50	100	84.5	73642	PASS
443	442	15	24	20.0	14751	PASS