


Data Path : Z:\HPCHEM1\BNA_F\Data\BF081617\
 Data File : BF097759.D
 Acq On : 17 Aug 2017 1:15
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 15 13:25:08 2017

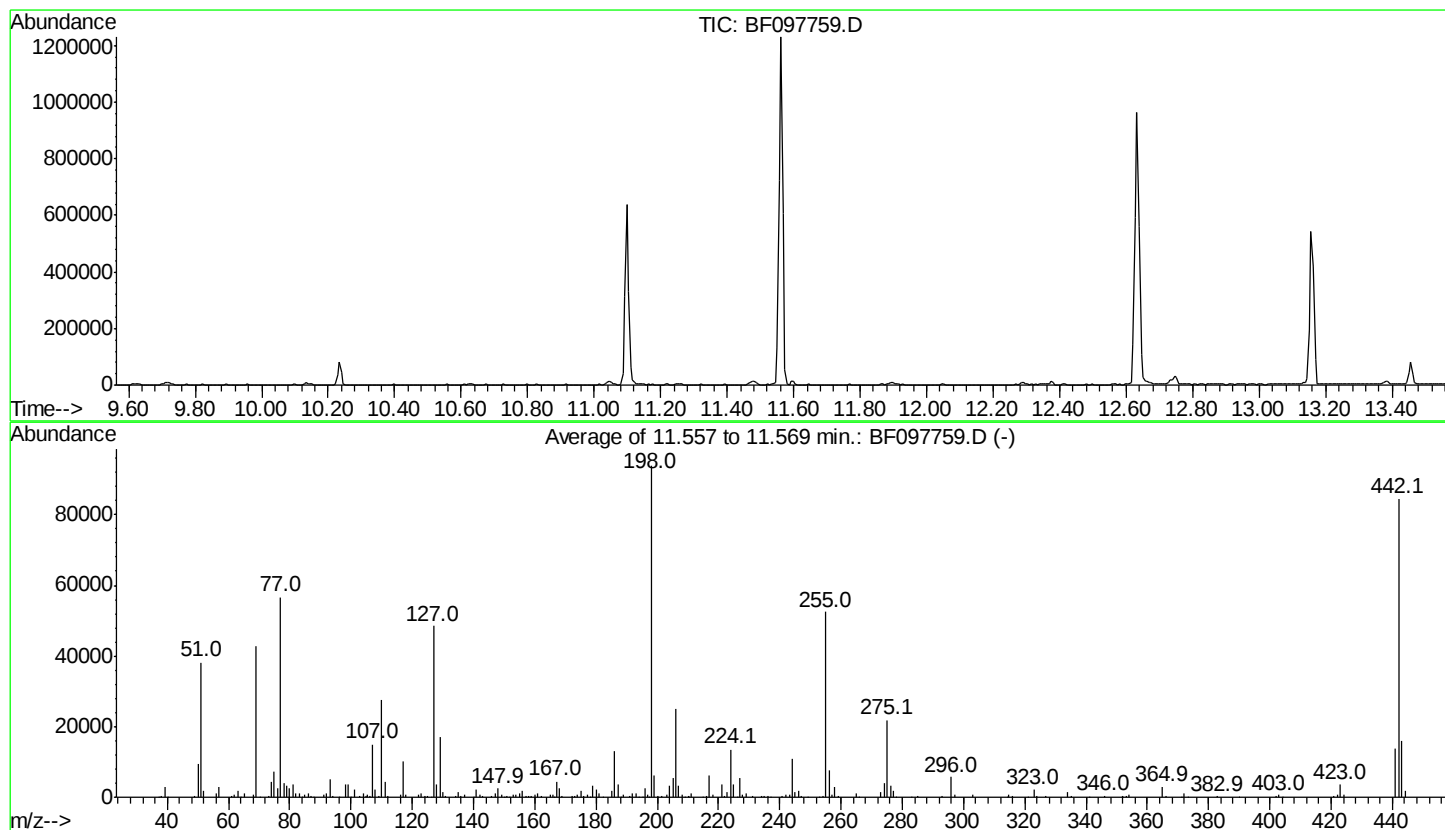

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	38237	PASS
68	69	0.00	2	1.3	560	PASS
69	198	0.00	100	45.5	42677	PASS
70	69	0.00	2	0.3	114	PASS
127	198	10	80	51.7	48538	PASS
197	198	0.00	2	0.9	841	PASS
198	198	100	100	100.0	93898	PASS
199	198	5	9	6.4	6031	PASS
275	198	10	60	23.2	21803	PASS
365	198	1	100	3.1	2930	PASS
441	442	0.01	24	16.2	13689	PASS
442	198	50	100	90.0	84517	PASS
443	442	15	24	18.8	15926	PASS