
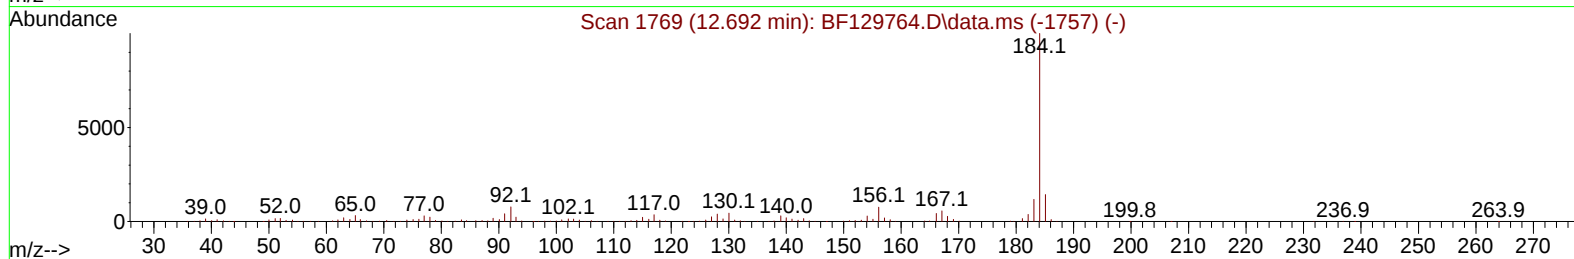
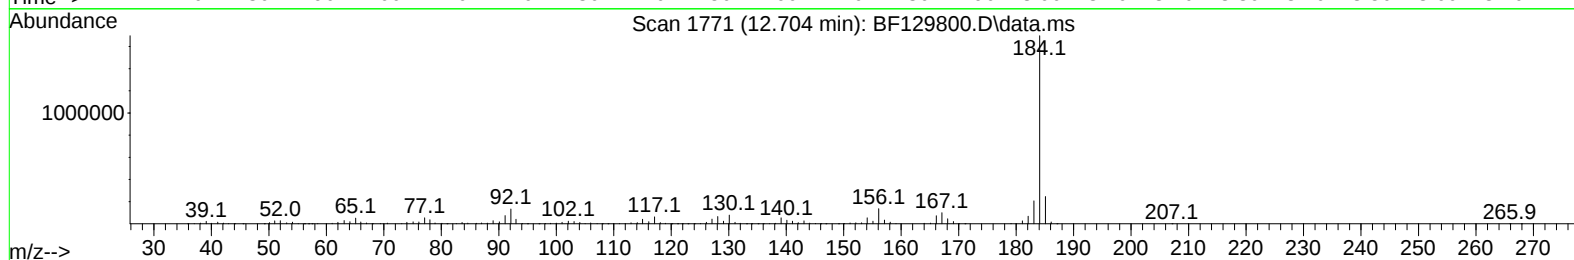


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081622\  
Data File : BF129800.D  
Acq On : 16 Aug 2022 08:50  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 07:30:51 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 15 02:28:31 2022  
Response via : Initial Calibration

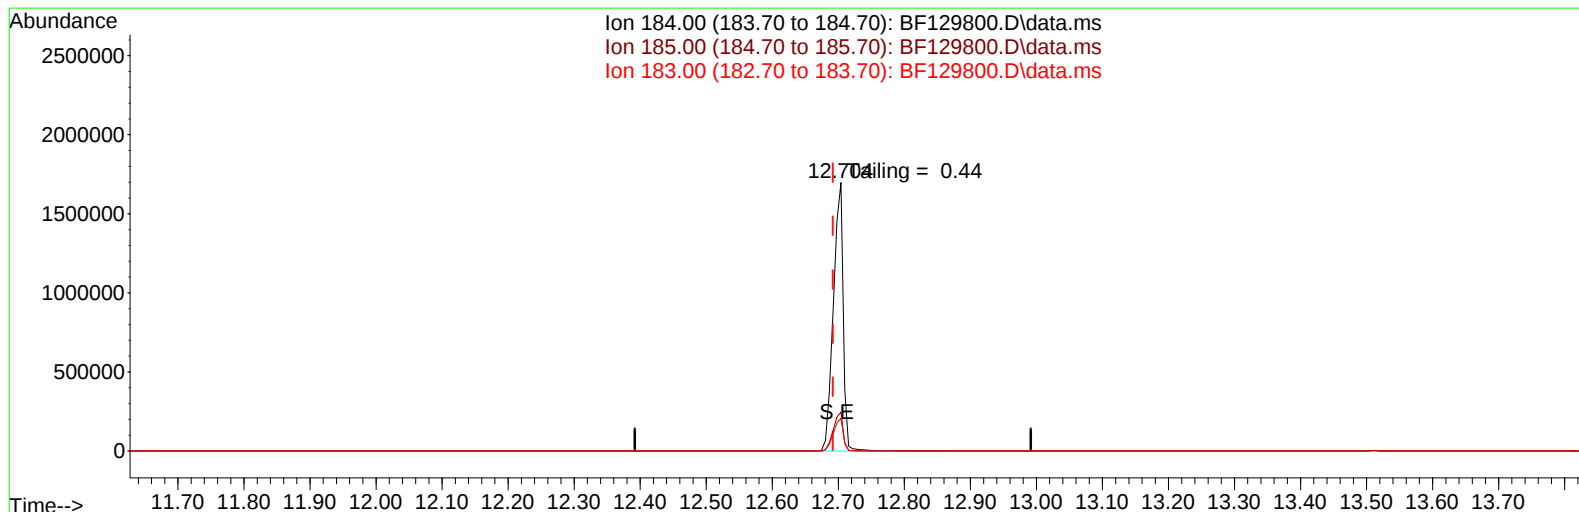

TIC: BF129800.D\data.ms

**(77) Benzidine**




12.704min (+ 0.012) 77377.39 ng

response 1755724

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 14.48  |
| 183.00 | 11.80  | 12.18  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081622\  
Data File : BF129800.D  
Acq On : 16 Aug 2022 08:50  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 07:30:51 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 15 02:28:31 2022  
Response via : Initial Calibration

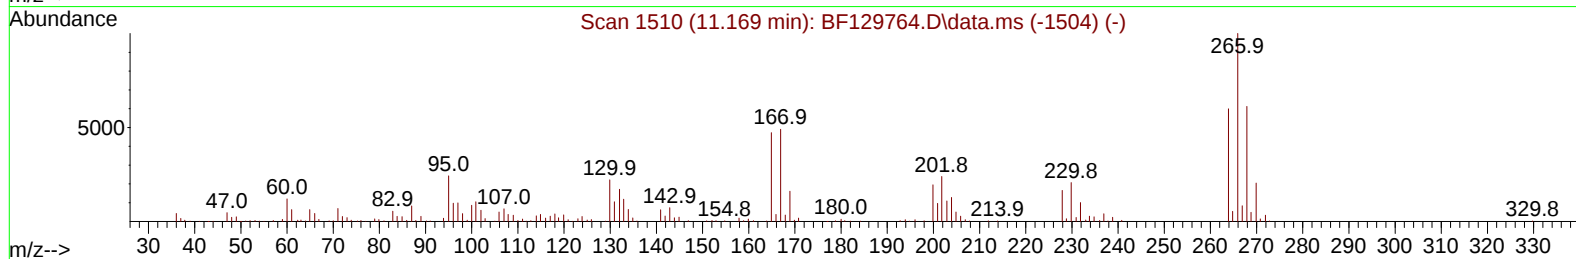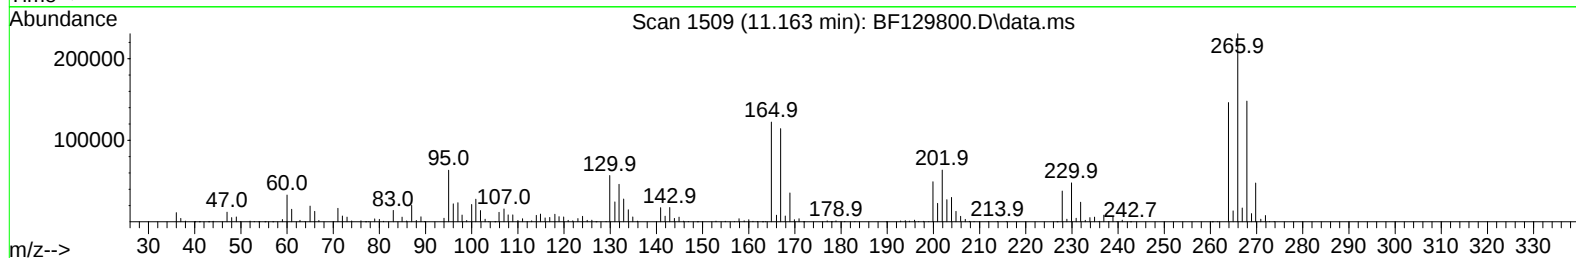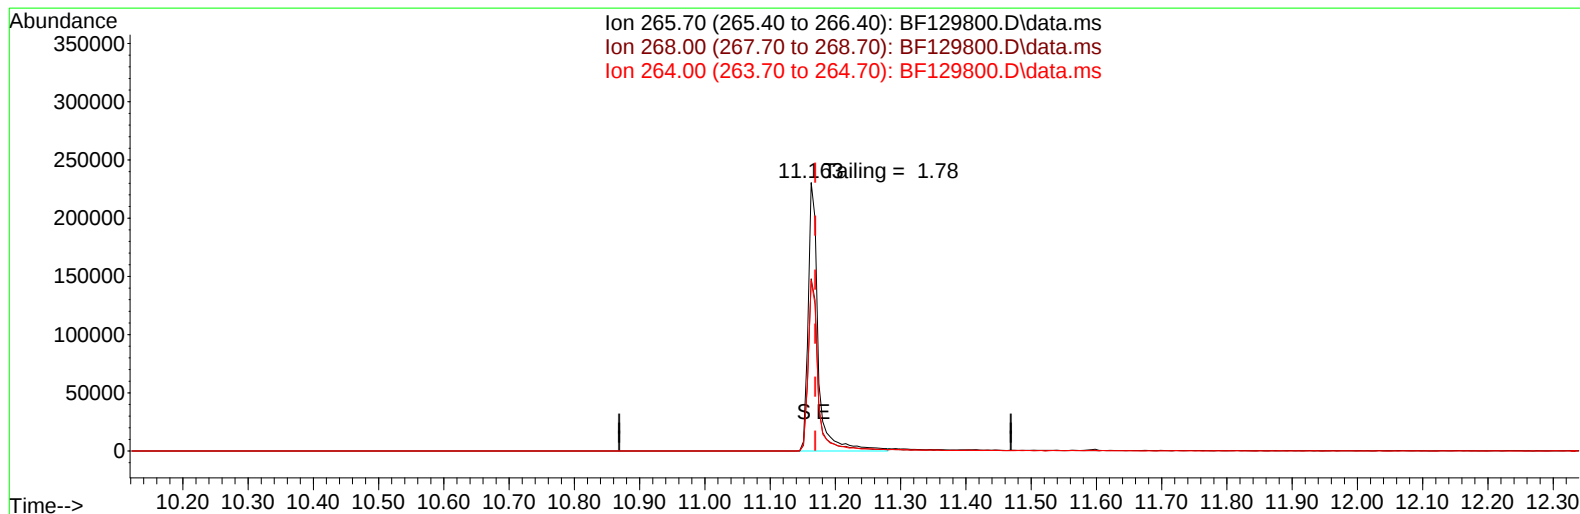

TIC: BF129800.D\data.ms

**(70) Pentachlorophenol (C)**

**11.163min (-0.006) 90056.04 ng**

**response 253038**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 64.16  |
| 264.00 | 59.90  | 63.46  |
| 0.00   | 0.00   | 0.00   |