
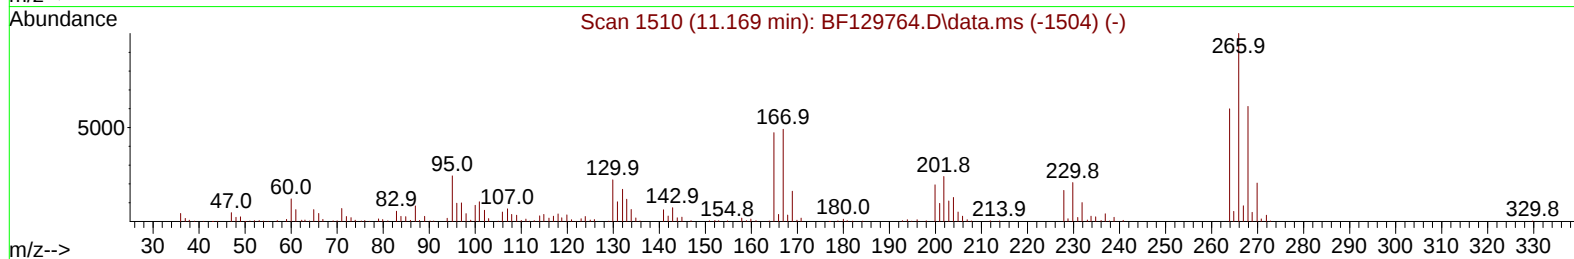
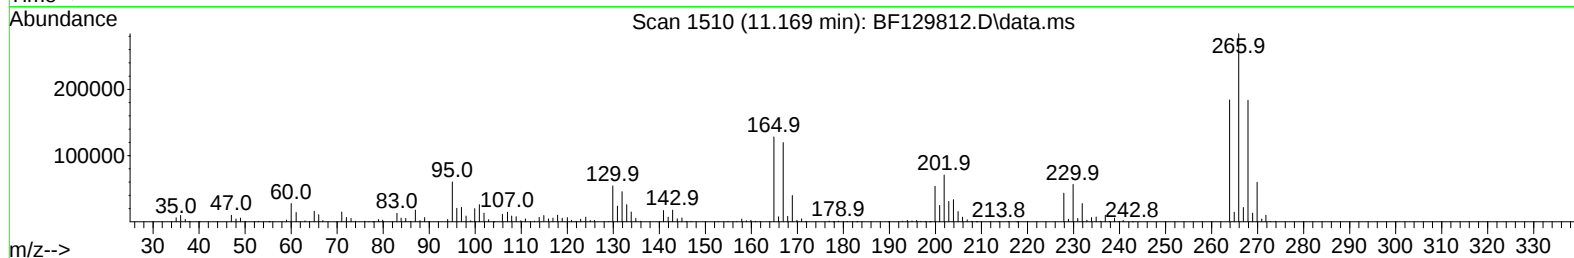


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129812.D
Acq On : 16 Aug 2022 15:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 07:36:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

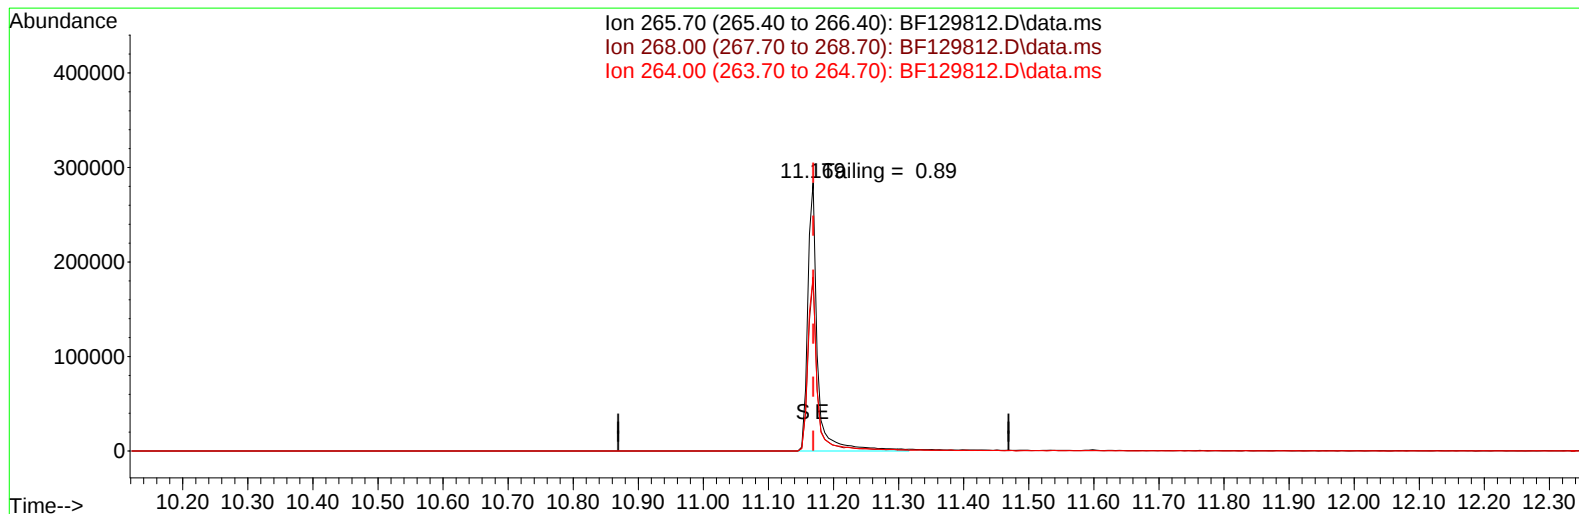

TIC: BF129812.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.000) 113135.79 ng

response 299029

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.59
264.00	59.90	64.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129812.D
Acq On : 16 Aug 2022 15:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 17 07:36:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

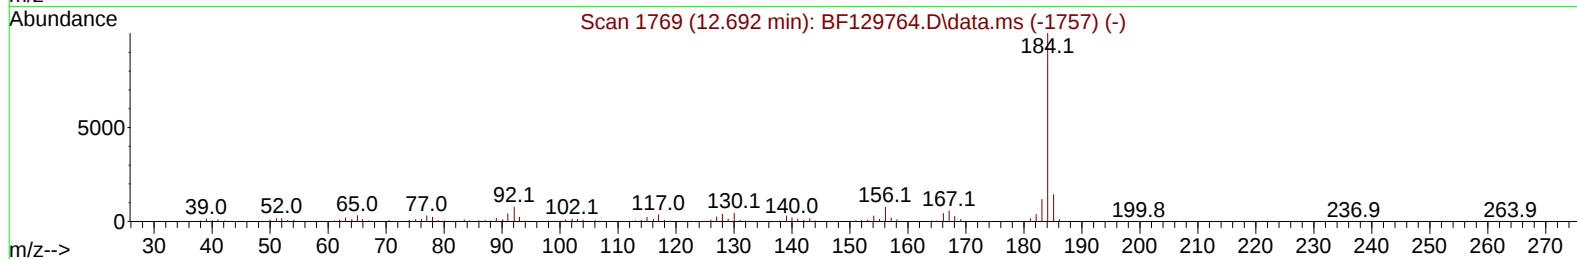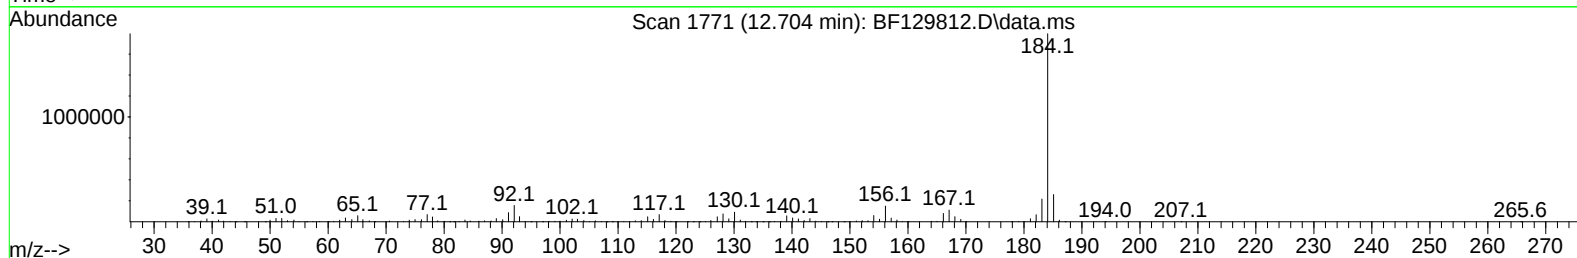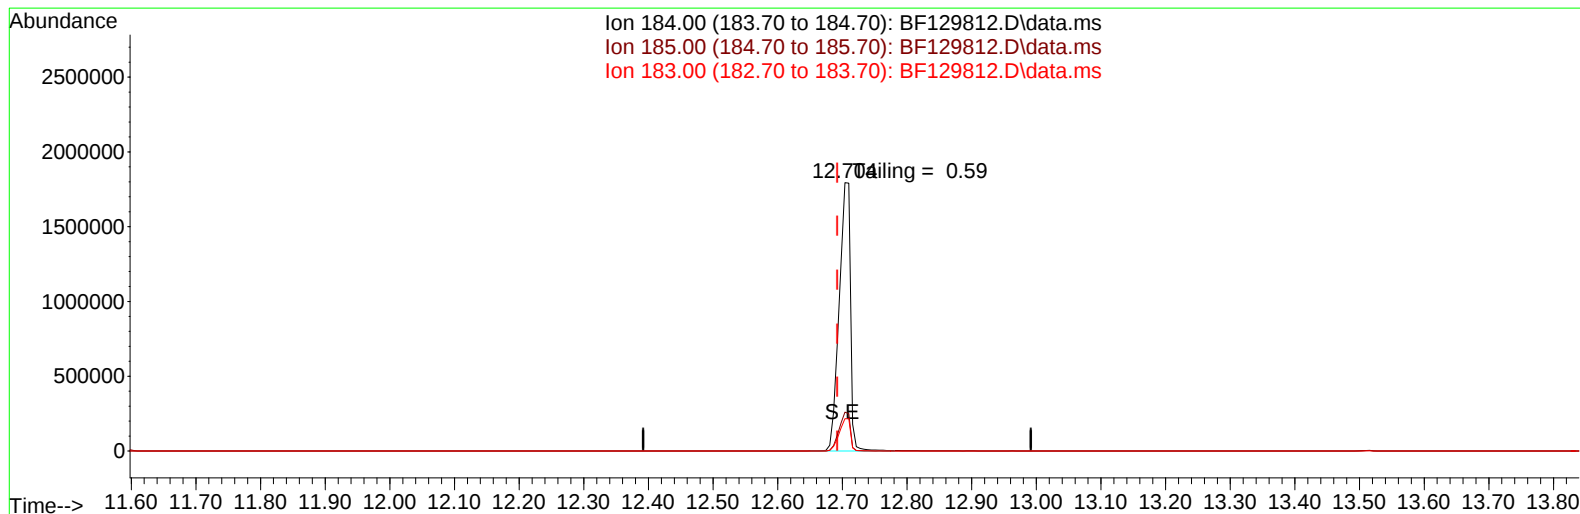

TIC: BF129812.D\data.ms

(77) Benzidine

12.704min (+ 0.012) 84522.76 ng

response 2184160

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.48
183.00	11.80	12.07
0.00	0.00	0.00