

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
 Data File : BF129817.D
 Acq On : 16 Aug 2022 18:38
 Operator : CG\JU
 Sample : N4208-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-1

Quant Time: Aug 17 02:36:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 15 02:28:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.822	152	146511	20.000	ng	0.00
21) Naphthalene-d8	8.104	136	594643	20.000	ng	0.00
39) Acenaphthene-d10	9.857	164	315766	20.000	ng	0.00
64) Phenanthrene-d10	11.351	188	524189	20.000	ng	0.00
76) Chrysene-d12	13.998	240	276393	20.000	ng	0.00
86) Perylene-d12	15.462	264	273991	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.463	112	521728	58.960	ng	0.00
7) Phenol-d6	6.475	99	687263	62.020	ng	0.00
23) Nitrobenzene-d5	7.386	82	455781	41.031	ng	-0.01
42) 2,4,6-Tribromophenol	10.651	330	164035	51.759	ng	-0.01
45) 2-Fluorobiphenyl	9.175	172	886590	42.644	ng	-0.01
79) Terphenyl-d14	12.933	244	813938	49.001	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129817.D
Acq On : 16 Aug 2022 18:38
Operator : CG\JU
Sample : N4208-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-1

Quant Time: Aug 17 02:36:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration




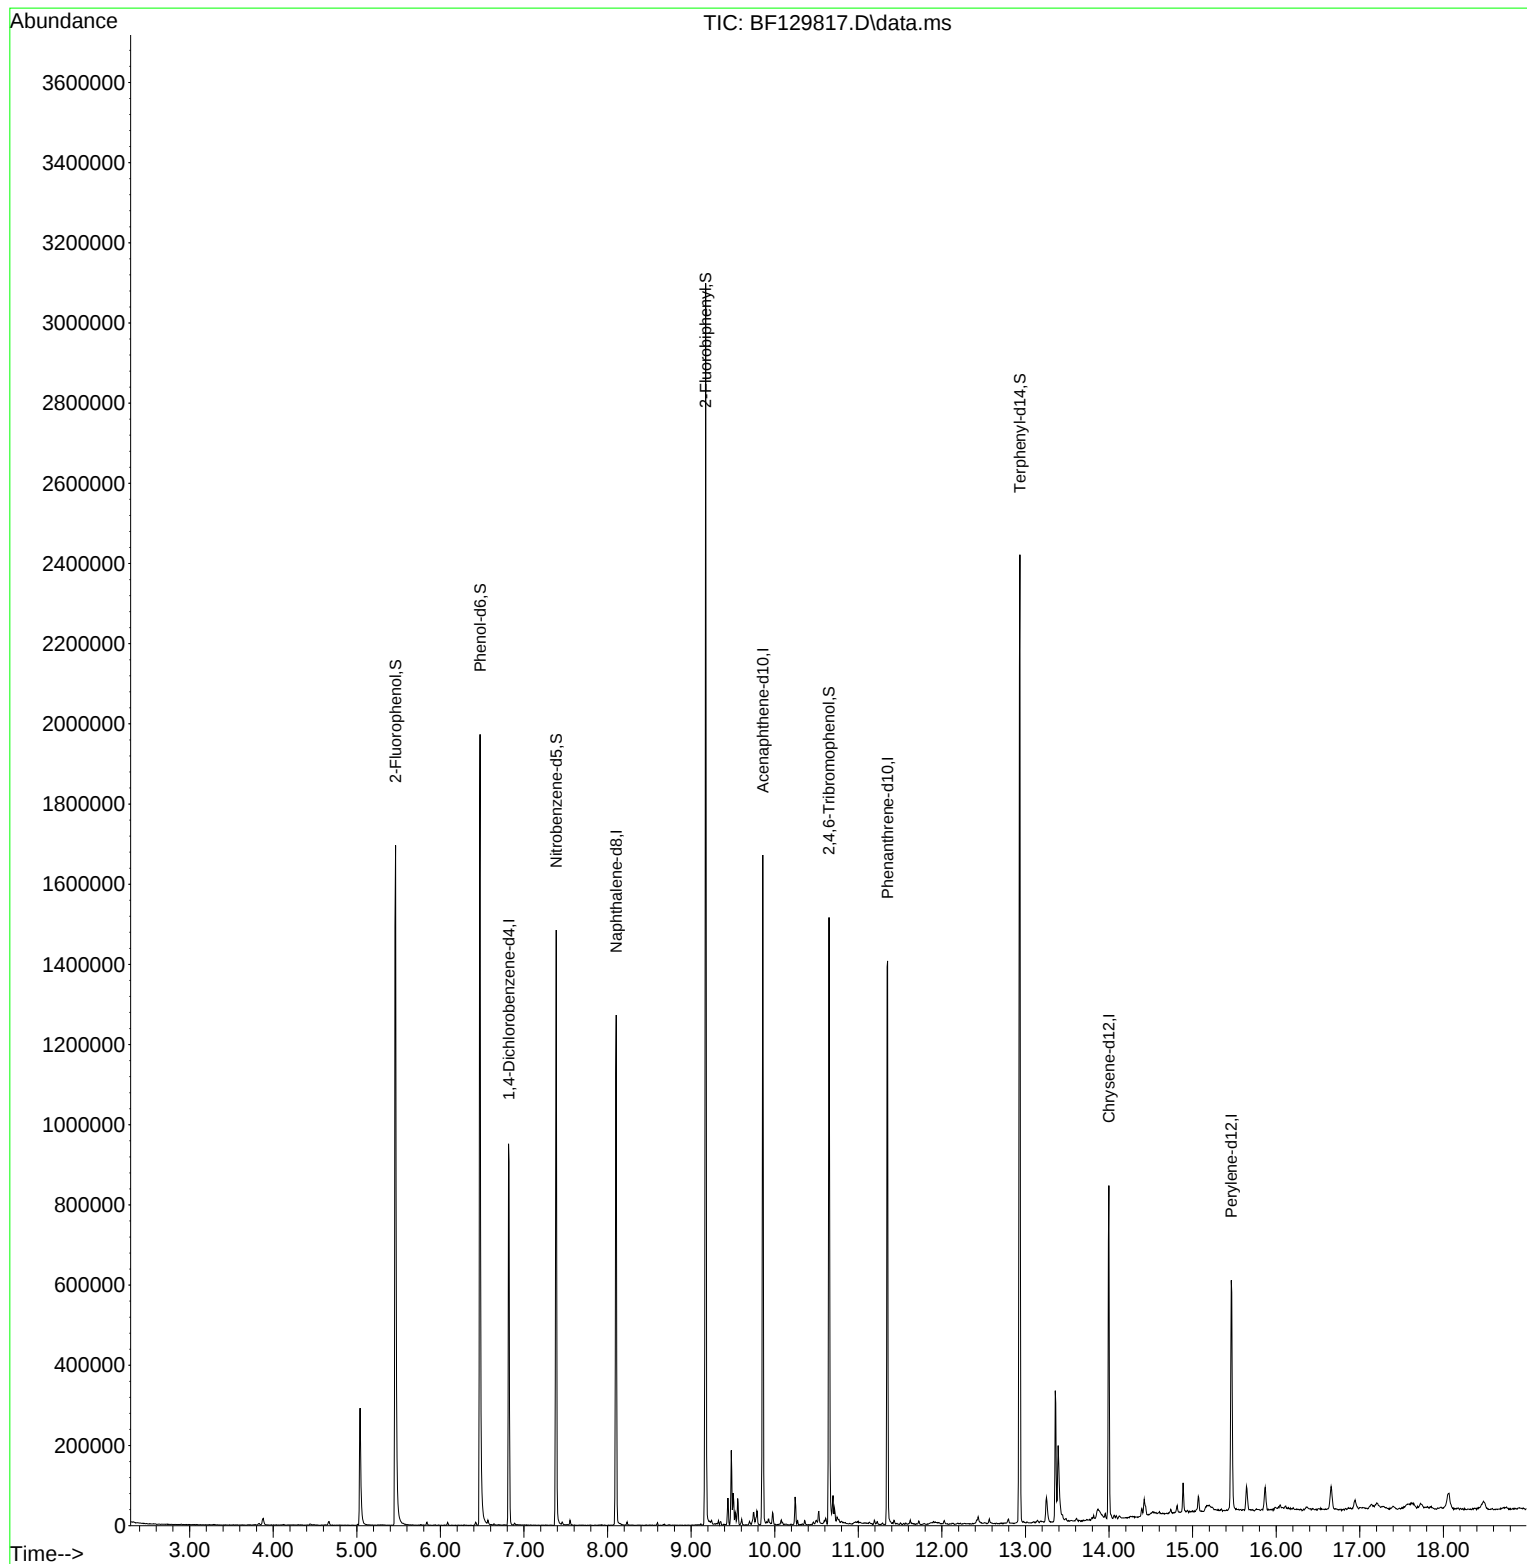


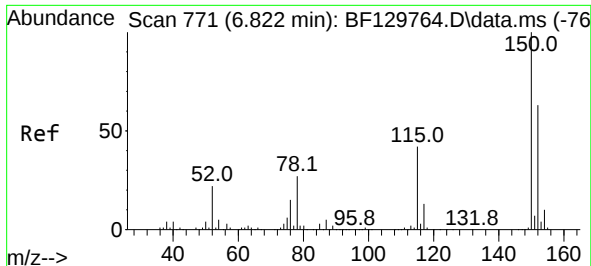

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.822 min Scan# 771
Delta R.T. -0.000 min
Lab File: BF129817.D
Acq: 16 Aug 2022 18:38




Instrument :
BNA_F
ClientSampleId :
W-1


Tgt Ion:152 Resp: 146511
Ion Ratio Lower Upper
152 100
150 154.5 126.9 190.3
115 60.8 53.4 80.0

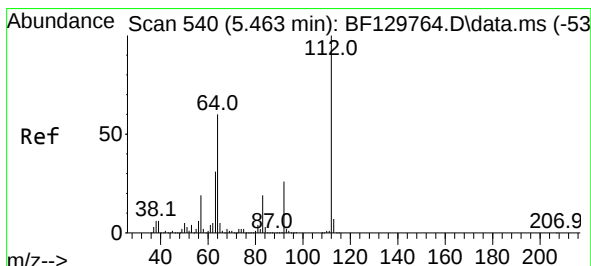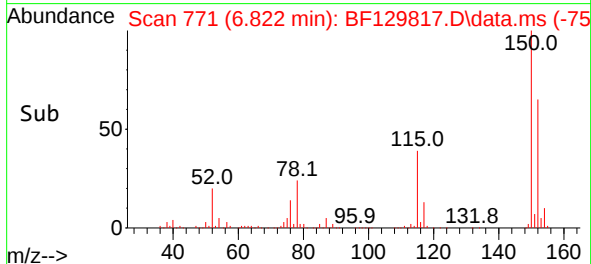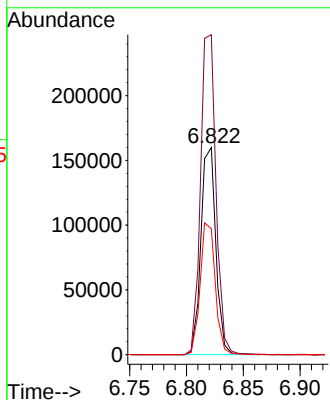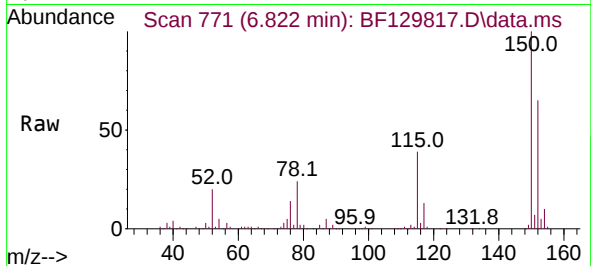

#5
2-Fluorophenol
Concen: 58.960 ng
RT: 5.463 min Scan# 540
Delta R.T. -0.000 min
Lab File: BF129817.D
Acq: 16 Aug 2022 18:38

Tgt Ion:112 Resp: 521728
Ion Ratio Lower Upper
112 100
64 58.5 47.6 71.4
63 30.1 24.6 37.0


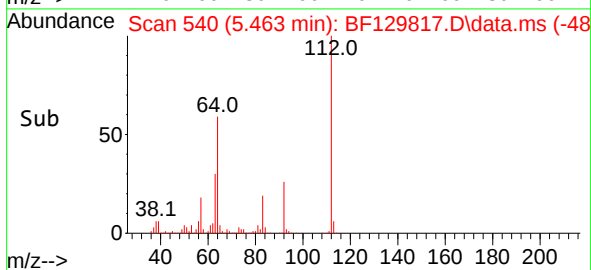
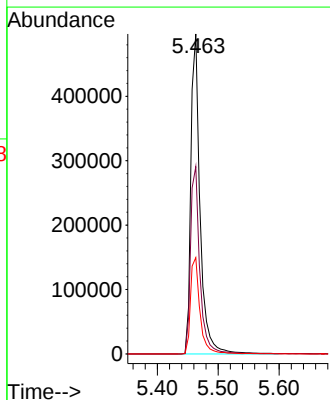
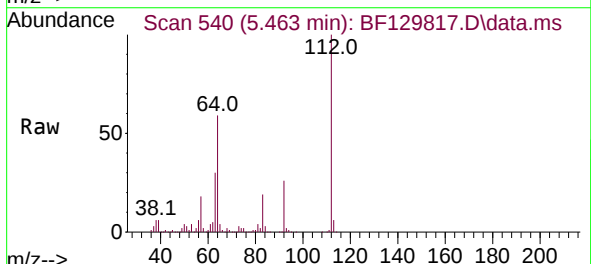


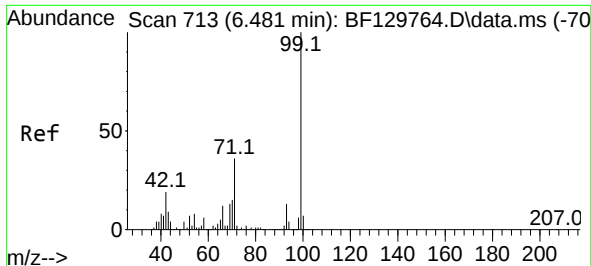

#7
Phenol-d6
Concen: 62.020 ng
RT: 6.475 min Scan# 713
Delta R.T. -0.006 min
Lab File: BF129817.D
Acq: 16 Aug 2022 18:38




Instrument :
BNA_F
ClientSampleId :
W-1


Tgt Ion: 99 Resp: 687263
Ion Ratio Lower Upper
99 100
42 17.0 15.0 22.4
71 34.4 28.8 43.2

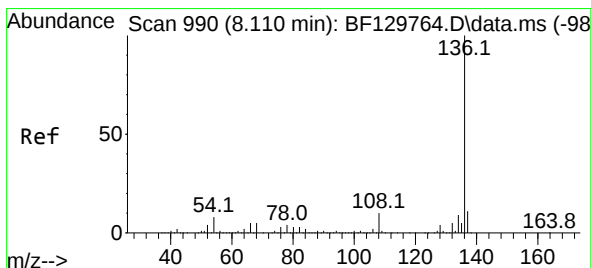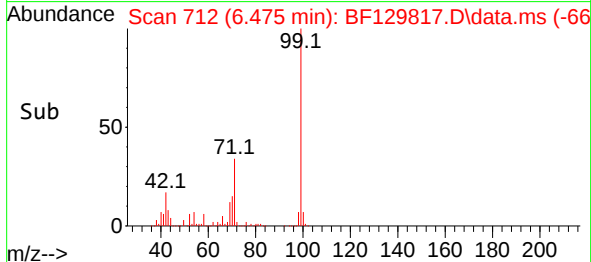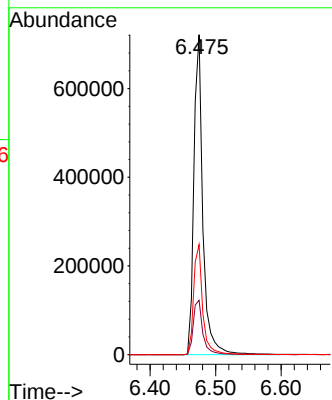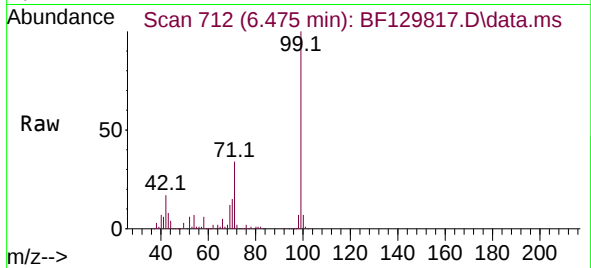

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.104 min Scan# 989
Delta R.T. -0.006 min
Lab File: BF129817.D
Acq: 16 Aug 2022 18:38

Tgt Ion: 136 Resp: 594643
Ion Ratio Lower Upper
136 100
137 10.8 8.4 12.6
54 7.3 6.2 9.2
68 5.1 4.2 6.4

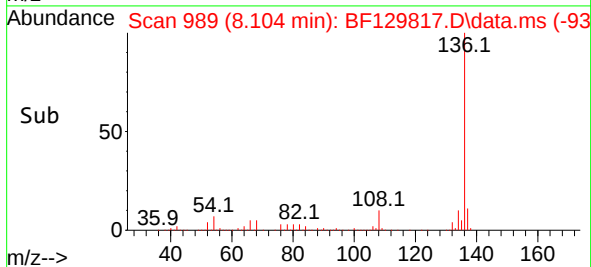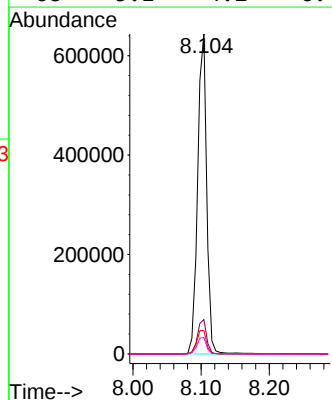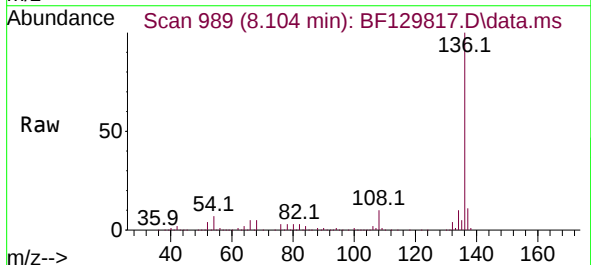

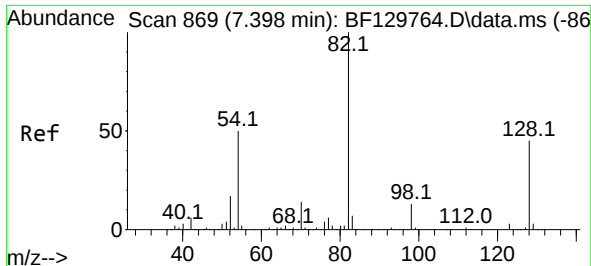

#23

Nitrobenzene-d5

Concen: 41.031 ng

RT: 7.386 min Scan# 867

Delta R.T. -0.012 min

Lab File: BF129817.D

Acq: 16 Aug 2022 18:38

Instrument :

BNA_F

ClientSampleId :

W-1





Tgt Ion: 82 Resp: 455781

Ion Ratio Lower Upper

82 100

128 43.6 36.1 54.1

54 50.3 40.0 60.0

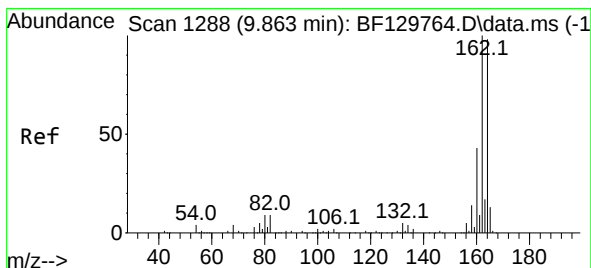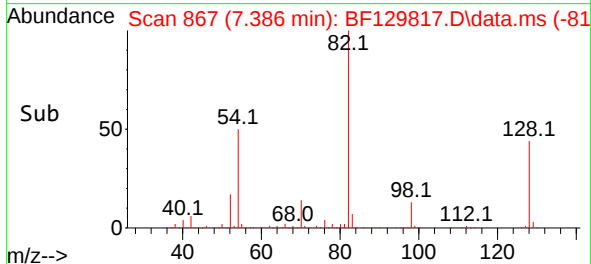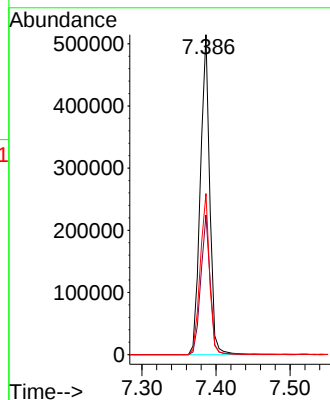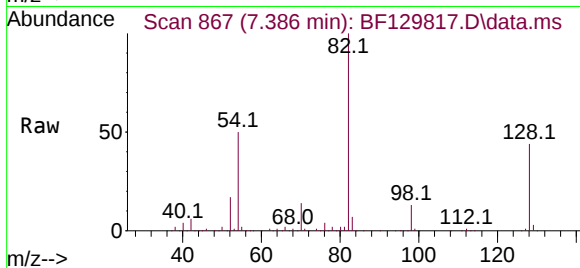

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.857 min Scan# 1287

Delta R.T. -0.006 min

Lab File: BF129817.D

Acq: 16 Aug 2022 18:38




Tgt Ion: 164 Resp: 315766


Ion Ratio Lower Upper

164 100

162 101.0 82.0 123.0

160 44.5 35.4 53.0

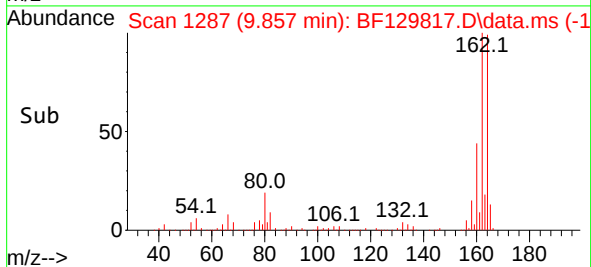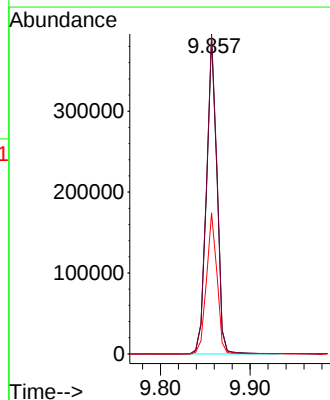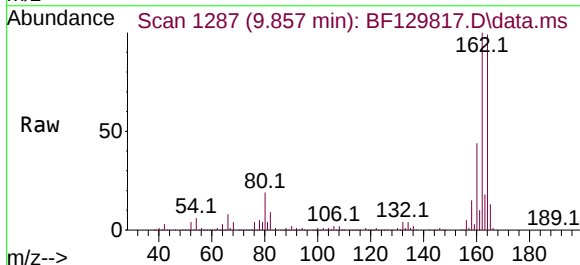

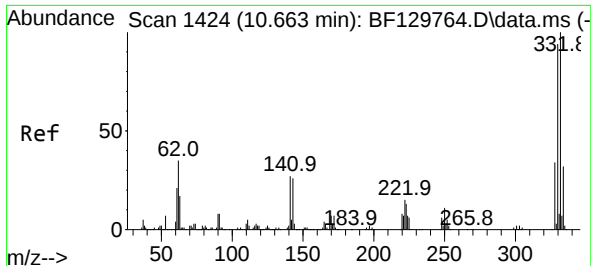

#42

2,4,6-Tribromophenol

Concen: 51.759 ng

RT: 10.651 min Scan# 1422

Delta R.T. -0.012 min

Lab File: BF129817.D

Acq: 16 Aug 2022 18:38

Instrument :

BNA_F

ClientSampleId :

W-1





Tgt Ion:330 Resp: 164035

Ion Ratio Lower Upper

330 100

332 101.3 82.6 124.0

141 35.4 27.6 41.4

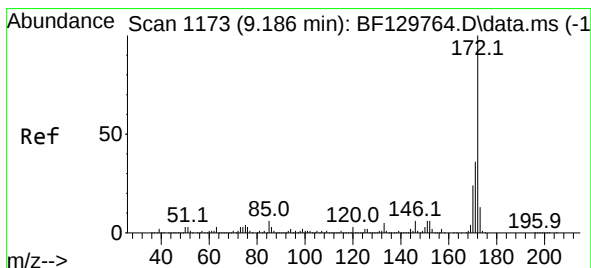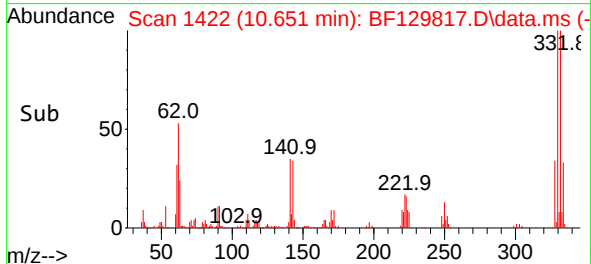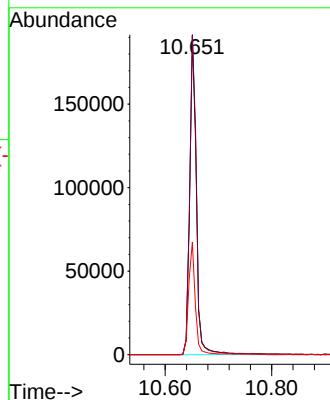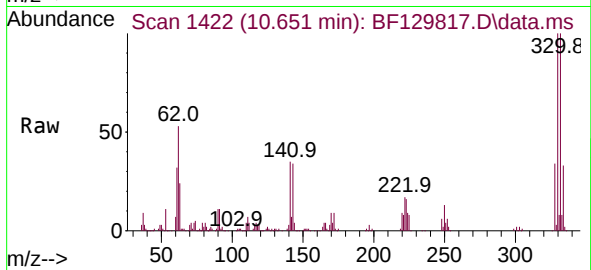

#45

2-Fluorobiphenyl

Concen: 42.644 ng

RT: 9.175 min Scan# 1171

Delta R.T. -0.012 min

Lab File: BF129817.D

Acq: 16 Aug 2022 18:38




Tgt Ion:172 Resp: 886590


Ion Ratio Lower Upper

172 100

171 35.2 28.4 42.6

170 23.1 19.1 28.7


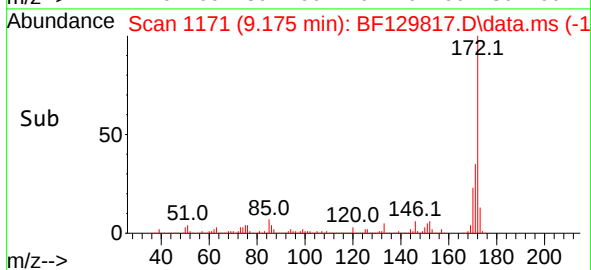
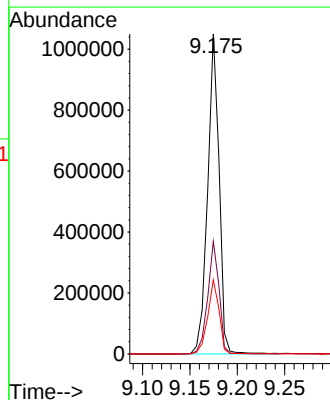
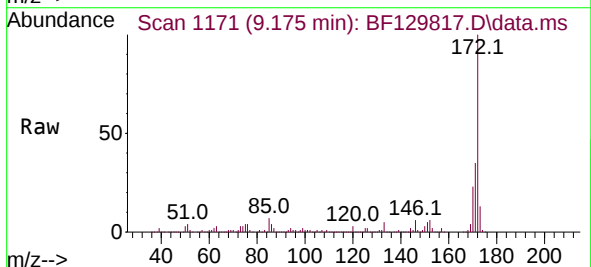


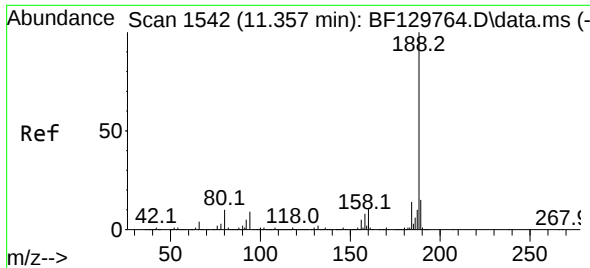

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.351 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF129817.D
Acq: 16 Aug 2022 18:38




Instrument :
BNA_F
ClientSampleId :
W-1


Tgt Ion:188 Resp: 524189
Ion Ratio Lower Upper
188 100
94 8.1 7.4 11.2
80 9.2 7.9 11.9

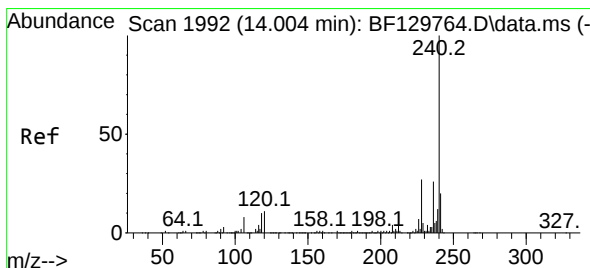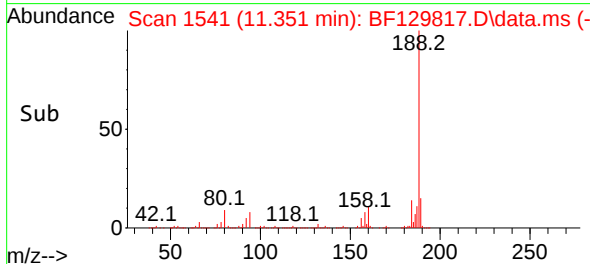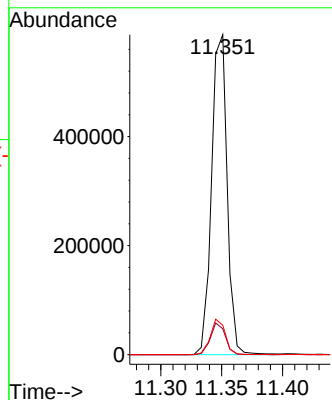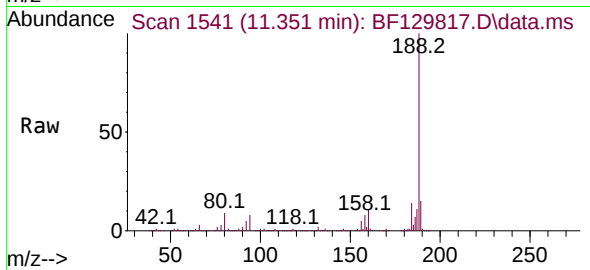

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.998 min Scan# 1991
Delta R.T. -0.006 min
Lab File: BF129817.D
Acq: 16 Aug 2022 18:38

Tgt Ion:240 Resp: 276393
Ion Ratio Lower Upper
240 100
120 10.7 9.2 13.8
236 24.9 20.7 31.1


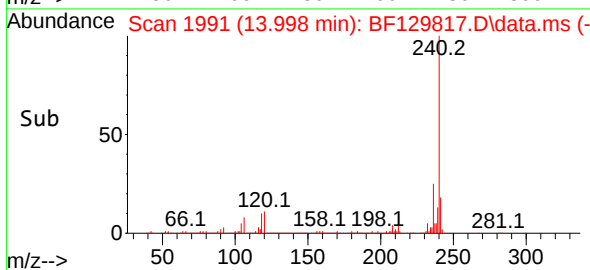
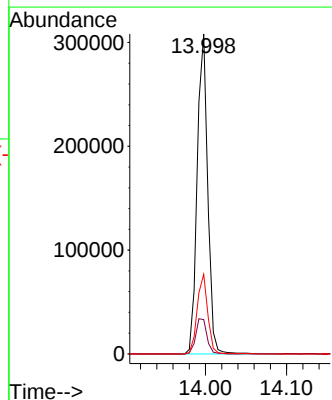
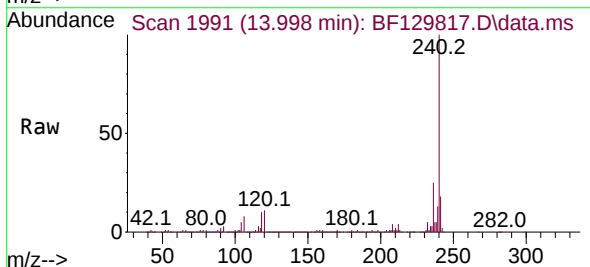


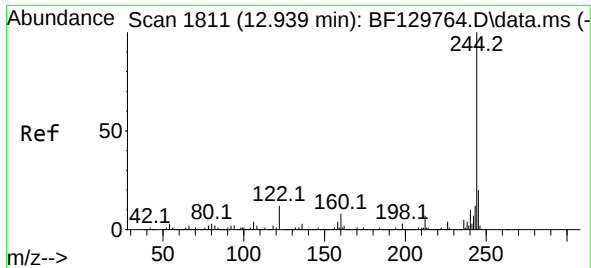

#79
 Terphenyl-d14
 Concen: 49.001 ng
 RT: 12.933 min Scan# 1811
 Delta R.T. -0.006 min
 Lab File: BF129817.D
 Acq: 16 Aug 2022 18:38

Instrument :
 BNA_F
 ClientSampleId :
 W-1

Tgt Ion:244 Resp: 813938
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.9 8.9
 122 10.8 9.9 14.9

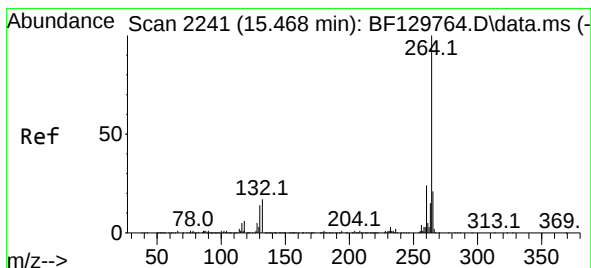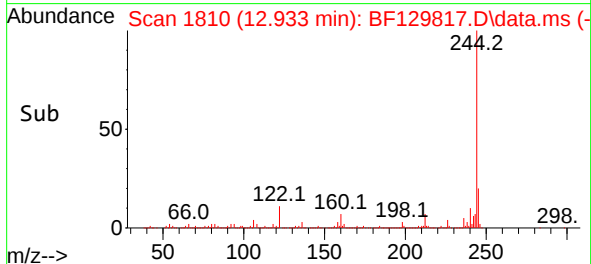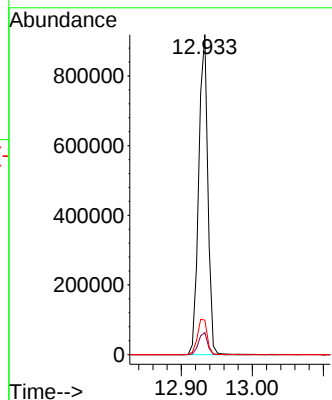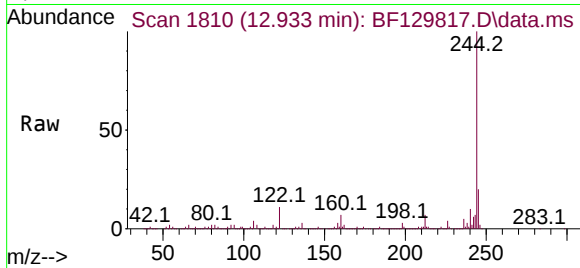

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.462 min Scan# 2240
 Delta R.T. -0.006 min
 Lab File: BF129817.D
 Acq: 16 Aug 2022 18:38

Tgt Ion:264 Resp: 273991
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.1 28.7
 265 21.5 16.7 25.1

