

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
 Data File : BF129805.D
 Acq On : 16 Aug 2022 11:43
 Operator : CG\JU
 Sample : N4046-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BEACONPOINT-BACKFILL-02

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129805.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	469	472	486	rVB	64578	90454	1.79%	0.291%
2	5.463	536	540	564	rBV	3982461	3720686	73.50%	11.988%
3	6.475	708	712	715	rBV	3748932	3785334	74.78%	12.197%
4	6.822	767	771	781	rVB	1065724	950647	18.78%	3.063%
5	7.392	862	868	871	rBV	2411376	2568453	50.74%	8.276%
6	8.104	984	989	992	rBV	1525953	1339993	26.47%	4.318%
7	9.181	1166	1172	1175	rBV	5565751	5062233	100.00%	16.311%
8	9.857	1280	1287	1291	rBV	1746612	1571586	31.05%	5.064%
9	10.657	1418	1423	1426	rBV	3564249	3116839	61.57%	10.043%
10	11.351	1537	1541	1544	rBV	1935311	1585087	31.31%	5.107%
11	11.728	1601	1605	1608	rVB	179813	137222	2.71%	0.442%
12	12.433	1719	1725	1728	rBV2	121320	112482	2.22%	0.362%
13	12.939	1806	1811	1814	rBV	5484489	4986785	98.51%	16.068%
14	13.886	1967	1972	1974	rBV4	41708	82522	1.63%	0.266%
15	13.998	1987	1991	1995	rBV	1177431	1037954	20.50%	3.344%
16	15.468	2235	2241	2253	rVB	685341	887457	17.53%	2.859%




Sum of corrected areas: 31035734

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129805.D
Acq On : 16 Aug 2022 11:43
Operator : CG\JU
Sample : N4046-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BEACONPOINT-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

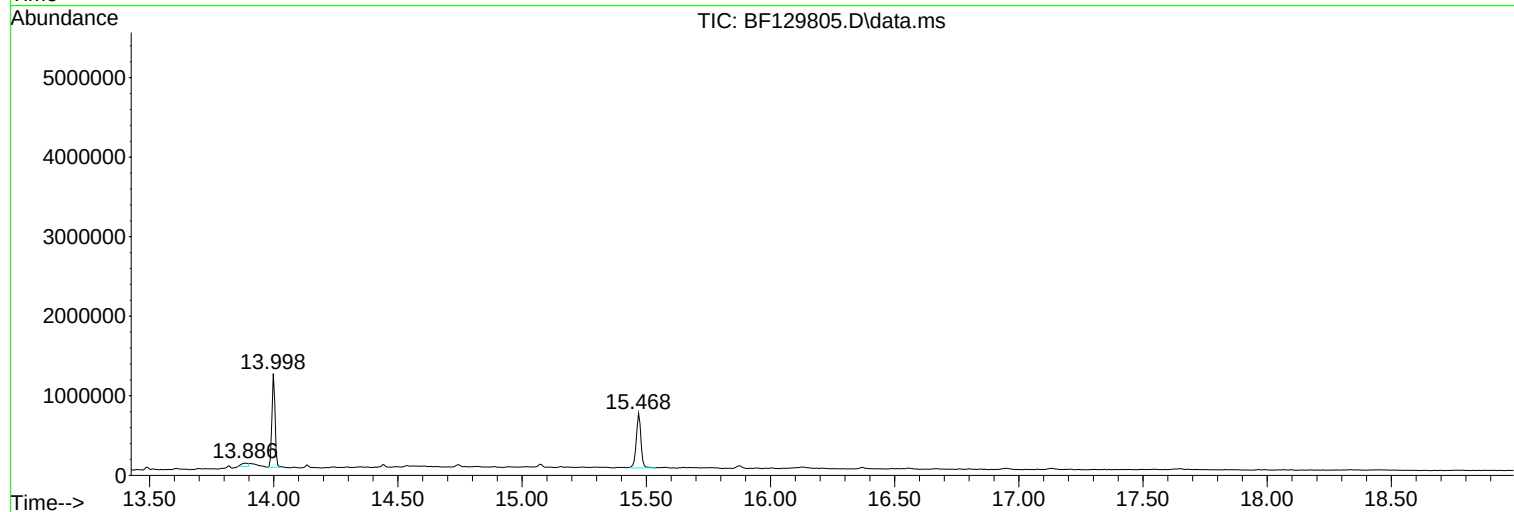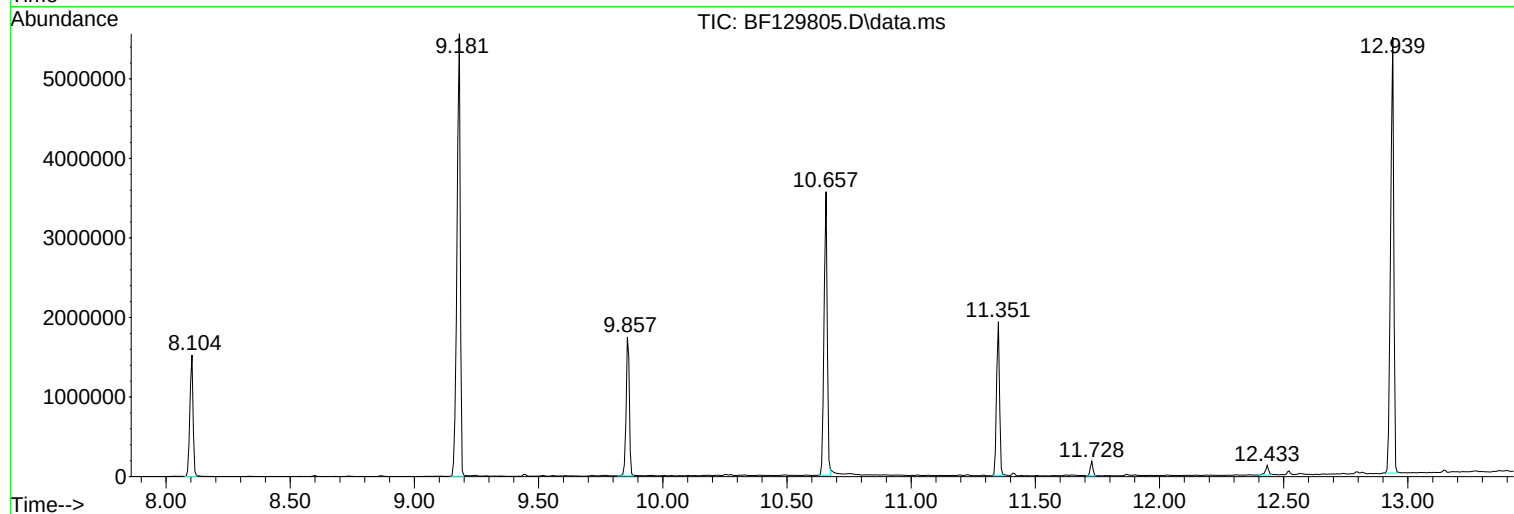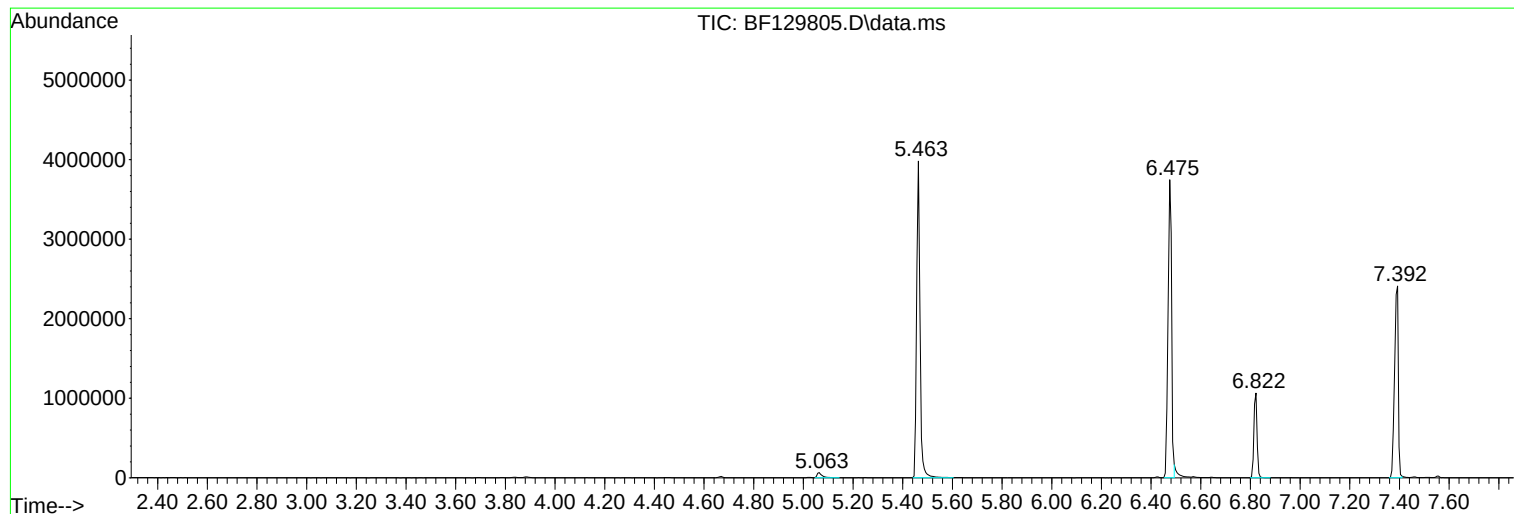

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129805.D
Acq On : 16 Aug 2022 11:43
Operator : CG\JU
Sample : N4046-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BEACONPOINT-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129805.D
Acq On : 16 Aug 2022 11:43
Operator : CG\JU
Sample : N4046-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BEACONPOINT-BACKFILL-02

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------