

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
 Data File : BF129832.D
 Acq On : 17 Aug 2022 02:38
 Operator : CG\JU
 Sample : N4218-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-081522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129832.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	536	539	557	rBV	1896280	1997168	19.59%	1.628%
2	6.475	709	712	726	rBV	2005993	1926608	18.90%	1.571%
3	6.822	767	771	775	rBV	954144	743817	7.30%	0.606%
4	7.386	863	867	872	rBV	1367881	1152626	11.31%	0.940%
5	8.104	986	989	991	rBV	1010451	957440	9.39%	0.781%
6	8.128	991	993	996	rVV	2909492	2146304	21.05%	1.750%
7	8.822	1107	1111	1114	rBV	1994152	1803587	17.69%	1.470%
8	8.916	1122	1127	1131	rVB	1704220	1479807	14.52%	1.206%
9	9.175	1165	1171	1175	rBV	2148879	1927922	18.91%	1.572%
10	9.280	1186	1189	1194	rBV	292404	245229	2.41%	0.200%
11	9.375	1203	1205	1211	rVB	234623	239905	2.35%	0.196%
12	9.445	1212	1217	1221	rBV	694580	910201	8.93%	0.742%
13	9.516	1225	1229	1232	rVV	1040944	1096192	10.75%	0.894%
14	9.545	1232	1234	1238	rVV	767330	646035	6.34%	0.527%
15	9.633	1246	1249	1255	rVB	524342	572015	5.61%	0.466%
16	9.722	1261	1264	1268	rBV2	1345474	1121624	11.00%	0.914%
17	9.839	1281	1284	1285	rBV	273993	212897	2.09%	0.174%
18	9.863	1285	1288	1290	rVV	870986	775523	7.61%	0.632%
19	9.892	1290	1293	1296	rVB	1730012	1545571	15.16%	1.260%
20	9.963	1302	1305	1309	rVB2	142856	192164	1.88%	0.157%
21	10.069	1318	1323	1325	rVV	1433165	1417342	13.90%	1.155%
22	10.098	1325	1328	1332	rVB2	349465	328875	3.23%	0.268%
23	10.175	1337	1341	1344	rBV	353983	409702	4.02%	0.334%
24	10.204	1344	1346	1352	rVB	278085	248074	2.43%	0.202%
25	10.269	1352	1357	1358	rBV2	208558	310964	3.05%	0.254%
26	10.410	1378	1381	1387	rVB	2744218	2740370	26.88%	2.234%
27	10.492	1393	1395	1398	rVV2	368308	340037	3.34%	0.277%
28	10.563	1405	1407	1410	rVB	427864	398059	3.90%	0.325%
29	10.657	1416	1423	1426	rBV3	1444482	1659884	16.28%	1.353%
30	10.769	1436	1442	1448	rVB4	164237	372933	3.66%	0.304%
31	10.957	1469	1474	1477	rVV2	667223	820184	8.05%	0.669%
32	10.986	1477	1479	1482	rVV	423461	371115	3.64%	0.303%
33	11.039	1485	1488	1491	rVV	362668	323545	3.17%	0.264%
34	11.086	1491	1496	1498	rVV2	195082	337561	3.31%	0.275%
35	11.110	1498	1500	1506	rVV2	251490	342093	3.36%	0.279%
36	11.163	1506	1509	1512	rVV	194875	229828	2.25%	0.187%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
 Data File : BF129832.D
 Acq On : 17 Aug 2022 02:38
 Operator : CG\JU
 Sample : N4218-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-081522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.198	1512	1515	1518	rVV2	304698	334912	3.29%	0.273%
38	11.251	1521	1524	1531	rVB	937159	876655	8.60%	0.715%
39	11.357	1538	1542	1543	rBV	715691	754520	7.40%	0.615%
40	11.392	1543	1548	1550	rVV	8882684	10071060	98.79%	8.210%
41	11.439	1550	1556	1559	rVV	3579615	3496248	34.30%	2.850%
42	11.463	1559	1560	1563	rVV	273756	247841	2.43%	0.202%
43	11.510	1565	1568	1574	rVV3	165853	259623	2.55%	0.212%
44	11.592	1576	1582	1586	rVV2	1296952	1416380	13.89%	1.155%
45	11.645	1589	1591	1595	rVV3	279313	338991	3.33%	0.276%
46	11.686	1595	1598	1602	rVV3	369525	470036	4.61%	0.383%
47	11.727	1602	1605	1608	rVV3	184789	202553	1.99%	0.165%
48	11.769	1608	1612	1616	rVB	259477	286794	2.81%	0.234%
49	11.857	1623	1627	1629	rBV	1714617	1519914	14.91%	1.239%
50	11.886	1629	1632	1635	rVB	2266964	1920893	18.84%	1.566%
51	11.933	1636	1640	1643	rBV	877453	834410	8.18%	0.680%
52	11.974	1643	1647	1649	rBV2	2694872	2923063	28.67%	2.383%
53	12.039	1655	1658	1660	rBV2	229180	230460	2.26%	0.188%
54	12.151	1674	1677	1680	rBV	995332	825010	8.09%	0.673%
55	12.186	1681	1683	1687	rVB2	433817	381681	3.74%	0.311%
56	12.298	1697	1702	1705	rBV2	309953	359942	3.53%	0.293%
57	12.333	1705	1708	1710	rVV	401825	314545	3.09%	0.256%
58	12.357	1710	1712	1715	rVB	282797	237904	2.33%	0.194%
59	12.410	1717	1721	1724	rBV	839830	1198485	11.76%	0.977%
60	12.445	1724	1727	1730	rVV2	628134	870431	8.54%	0.710%
61	12.510	1733	1738	1741	rBV2	398656	633493	6.21%	0.516%
62	12.592	1745	1752	1754	rBV	7482238	9628598	94.45%	7.850%
63	12.668	1762	1765	1769	rVB	388217	367346	3.60%	0.299%
64	12.727	1772	1775	1777	rBV2	426103	404765	3.97%	0.330%
65	12.821	1783	1791	1794	rBV2	7135038	10194611	100.00%	8.311%
66	12.851	1794	1796	1800	rVB2	536763	568711	5.58%	0.464%
67	12.939	1805	1811	1814	rVV2	2214427	2513855	24.66%	2.049%
68	12.968	1814	1816	1820	rVB	410970	362357	3.55%	0.295%
69	13.027	1820	1826	1829	rBV3	676914	1183794	11.61%	0.965%
70	13.057	1829	1831	1833	rVV	243570	238516	2.34%	0.194%
71	13.139	1837	1845	1850	rVV	1651594	2579094	25.30%	2.103%
72	13.204	1852	1856	1858	rVV	1652492	1627555	15.96%	1.327%
73	13.239	1858	1862	1865	rVV2	1037005	1346213	13.21%	1.097%
74	13.292	1869	1871	1874	rVV3	241114	244252	2.40%	0.199%
75	13.333	1875	1878	1880	rVV	626276	578124	5.67%	0.471%
76	13.363	1880	1883	1891	rVB2	738979	908126	8.91%	0.740%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
 Data File : BF129832.D
 Acq On : 17 Aug 2022 02:38
 Operator : CG\JU
 Sample : N4218-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OR-02-081522

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	13.533	1910	1912	1914	rBV	188522	189141	1.86%	0.154%
78	13.615	1923	1926	1929	rBV2	308735	382863	3.76%	0.312%
79	13.651	1929	1932	1935	rVB2	350565	357772	3.51%	0.292%
80	13.757	1947	1950	1952	rBV	496351	417261	4.09%	0.340%
81	13.780	1952	1954	1957	rVV	663190	556093	5.45%	0.453%
82	13.810	1957	1959	1965	rVV3	559542	896375	8.79%	0.731%
83	13.857	1965	1967	1974	rVB2	346269	506025	4.96%	0.413%
84	14.004	1987	1992	1996	rBV2	3576226	5146473	50.48%	4.196%
85	14.045	1996	1999	2004	rVB	3090943	3166773	31.06%	2.582%
86	14.115	2009	2011	2014	rBV	761373	667524	6.55%	0.544%
87	14.162	2017	2019	2024	rVB3	372439	393862	3.86%	0.321%
88	14.357	2050	2052	2054	rBV2	303073	303031	2.97%	0.247%
89	14.398	2056	2059	2062	rVV	678532	643330	6.31%	0.524%
90	14.427	2062	2064	2067	rVV2	244489	230700	2.26%	0.188%
91	14.498	2074	2076	2078	rVV	318114	260622	2.56%	0.212%
92	14.521	2078	2080	2082	rVV	332373	332317	3.26%	0.271%
93	14.545	2082	2084	2087	rVB2	482319	404573	3.97%	0.330%
94	15.062	2167	2172	2175	rBV	1931426	3290812	32.28%	2.683%
95	15.168	2187	2190	2194	rVB	642723	665440	6.53%	0.542%
96	15.368	2220	2224	2229	rVB	1162633	1388907	13.62%	1.132%
97	15.433	2230	2235	2239	rBV	1968558	2528464	24.80%	2.061%
98	15.521	2247	2250	2256	rVB	666984	859253	8.43%	0.700%
99	16.986	2493	2499	2506	rVB	823680	1648763	16.17%	1.344%
100	17.439	2571	2576	2586	rVB	596235	1332081	13.07%	1.086%


Sum of corrected areas: 122663417

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129832.D
Acq On : 17 Aug 2022 02:38
Operator : CG\JU
Sample : N4218-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

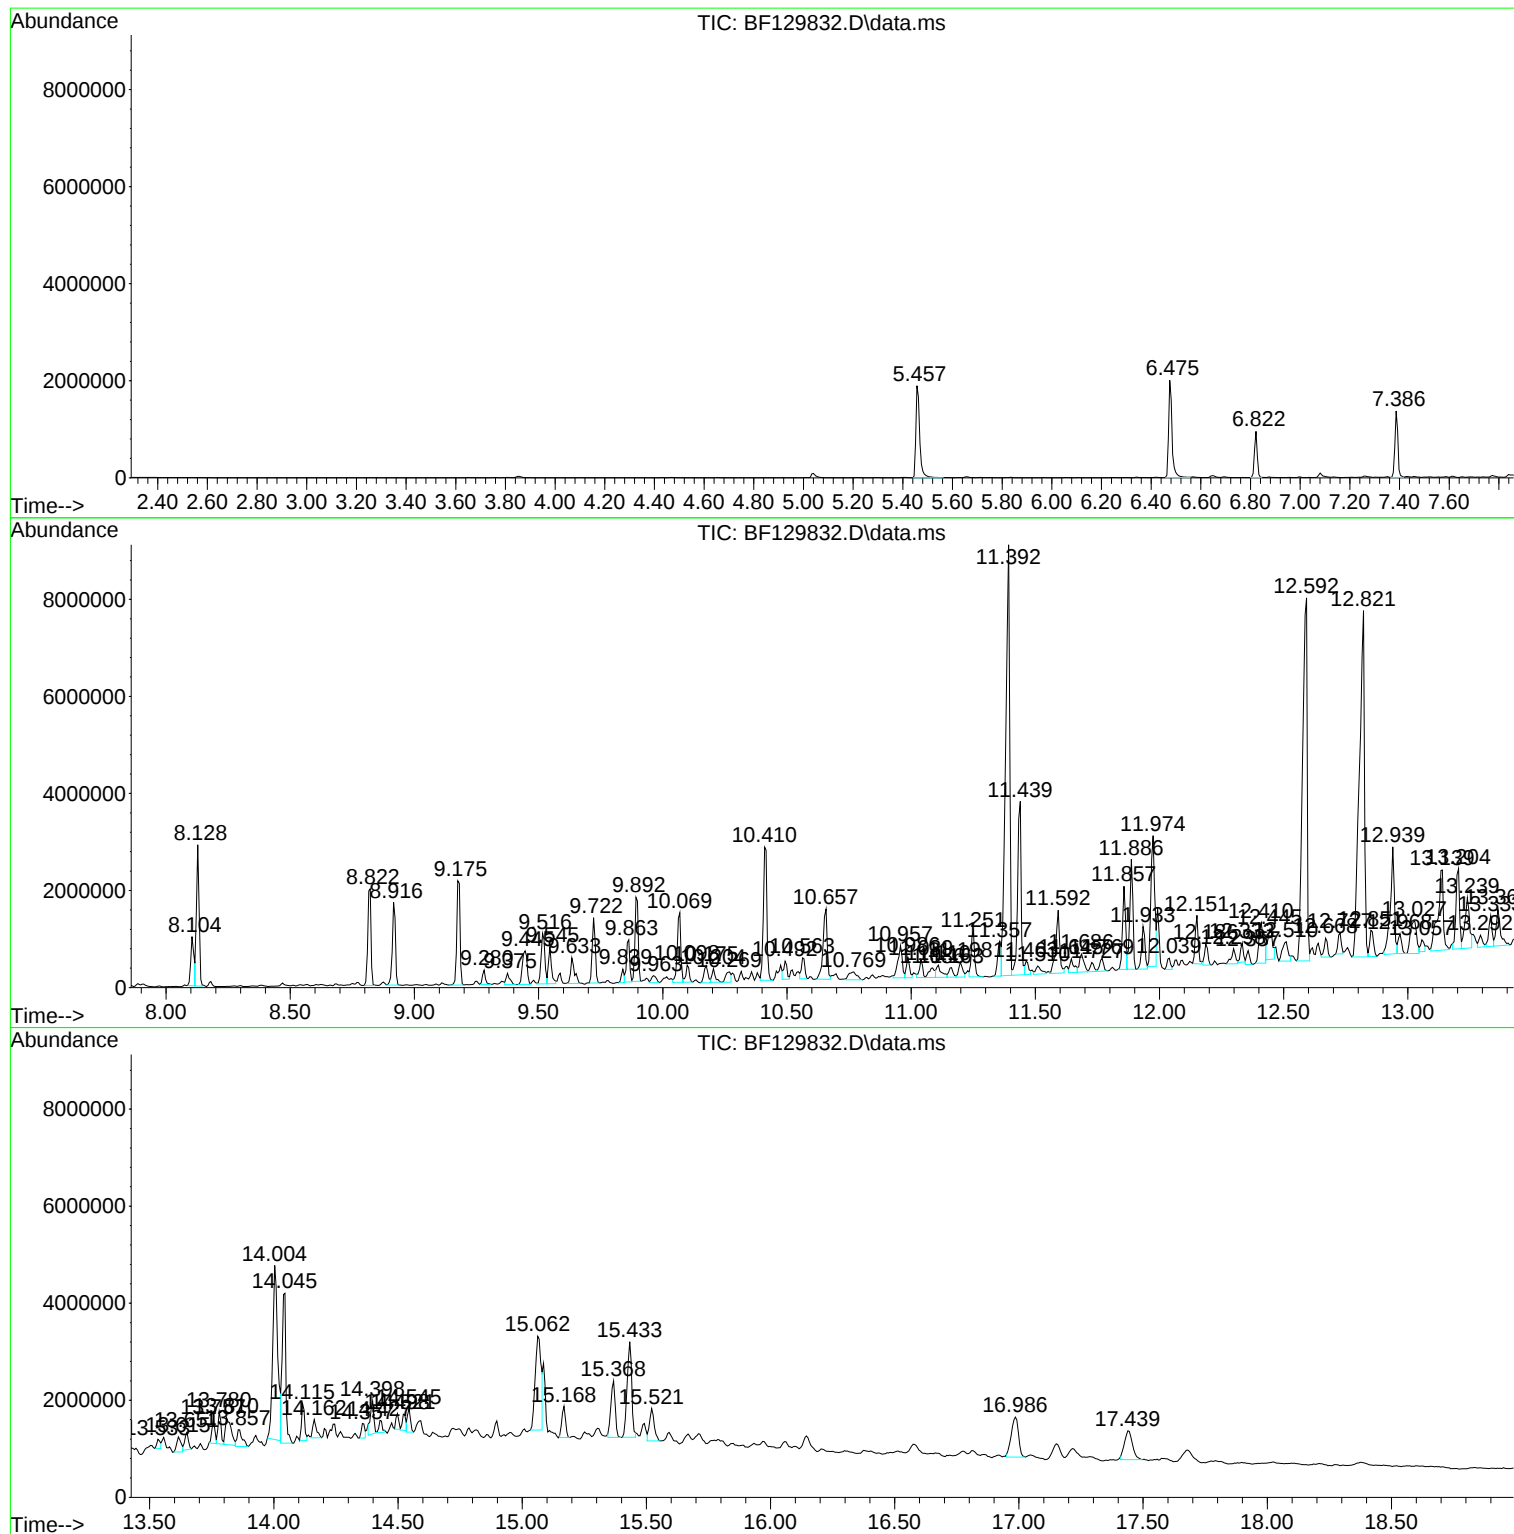

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129832.D
Acq On : 17 Aug 2022 02:38
Operator : CG\JU
Sample : N4218-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129832.D
Acq On : 17 Aug 2022 02:38
Operator : CG\JU
Sample : N4218-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OR-02-081522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------