


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
 Data File : BF129812.D
 Acq On : 16 Aug 2022 15:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 15 02:28:31 2022

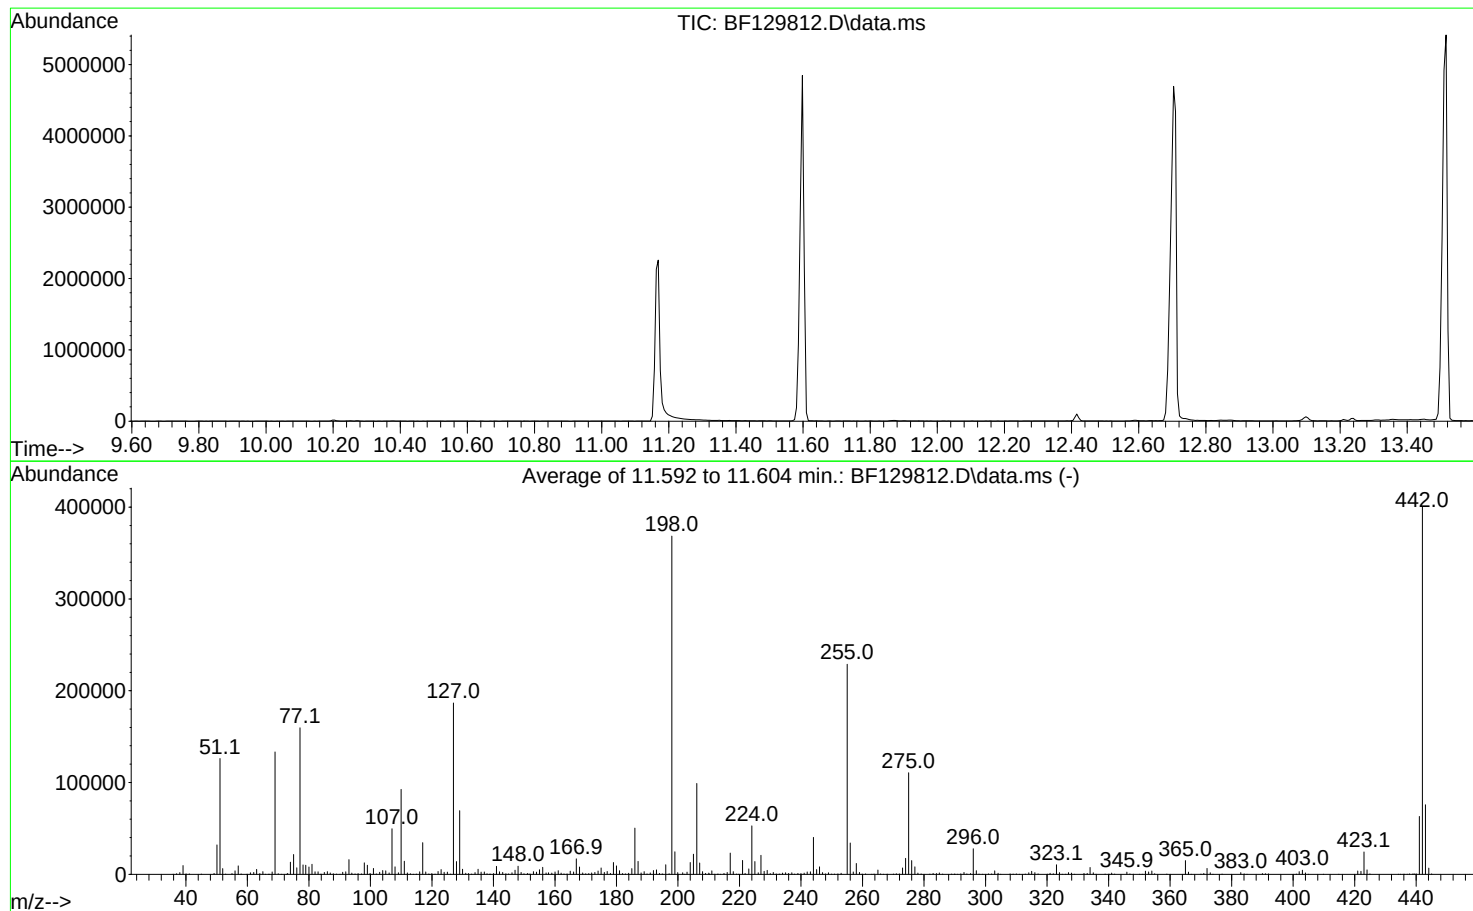




AutoFind: Scans 1582, 1583, 1584; Background Corrected with Scan 1575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	126083	PASS
68	69	0.00	2	1.9	2539	PASS
69	198	0.00	100	36.2	133317	PASS
70	69	0.00	2	0.5	641	PASS
127	198	10	80	50.6	186560	PASS
197	198	0.00	2	0.1	544	PASS
198	198	100	100	100.0	368427	PASS
199	198	5	9	6.7	24583	PASS
275	198	10	60	30.0	110629	PASS
365	198	1	100	4.1	14987	PASS
441	198	0.01	100	17.1	63083	PASS
442	442	50	100	100.0	400789	PASS
443	442	15	24	18.9	75675	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129812.D
Acq On : 16 Aug 2022 15:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 07:36:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

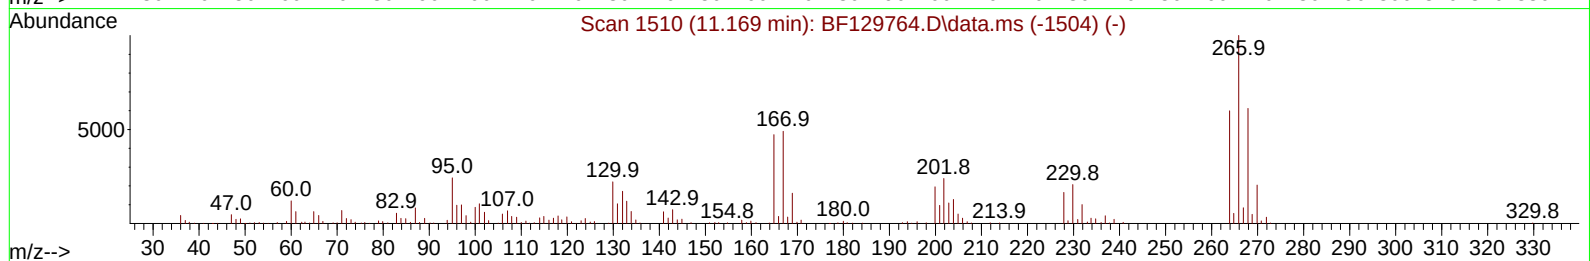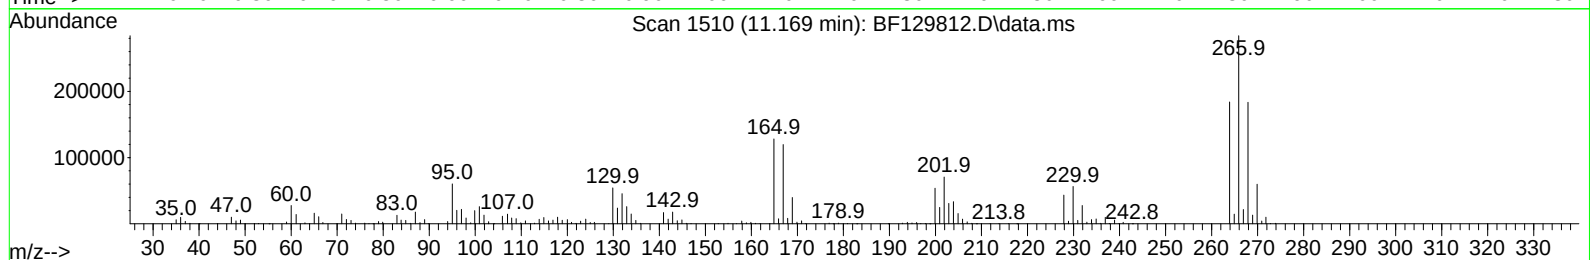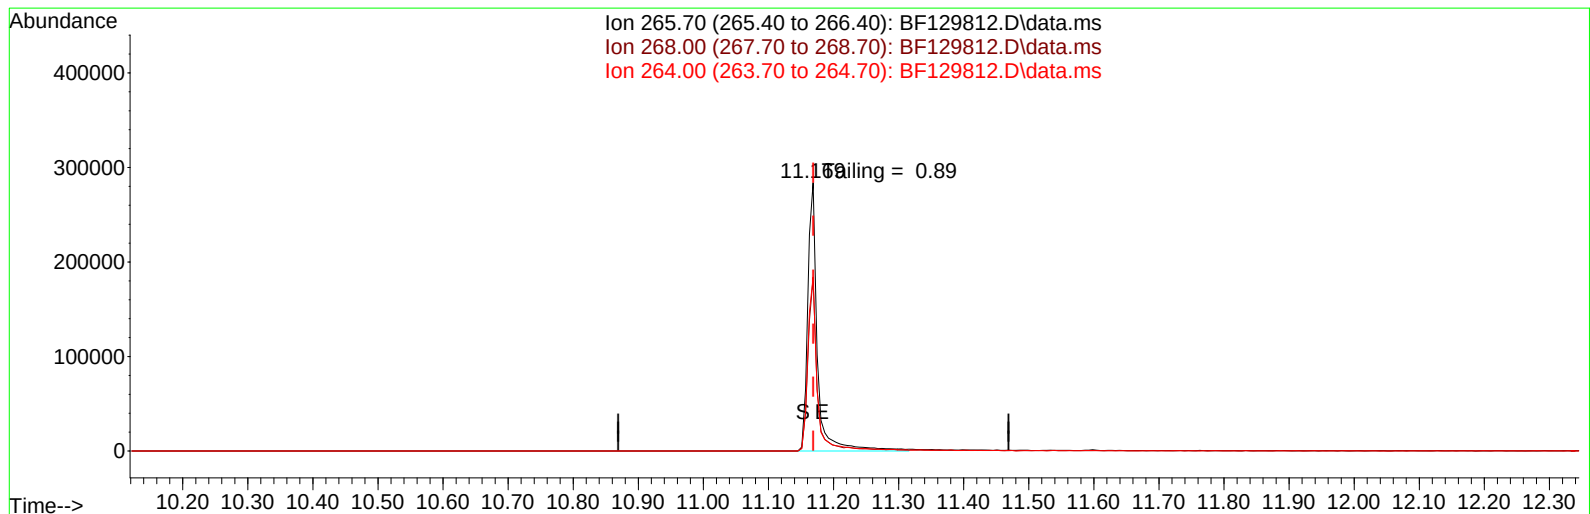

TIC: BF129812.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.000) 113135.79 ng




response 299029

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.59
264.00	59.90	64.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081622\
Data File : BF129812.D
Acq On : 16 Aug 2022 15:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 17 07:36:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 15 02:28:31 2022
Response via : Initial Calibration

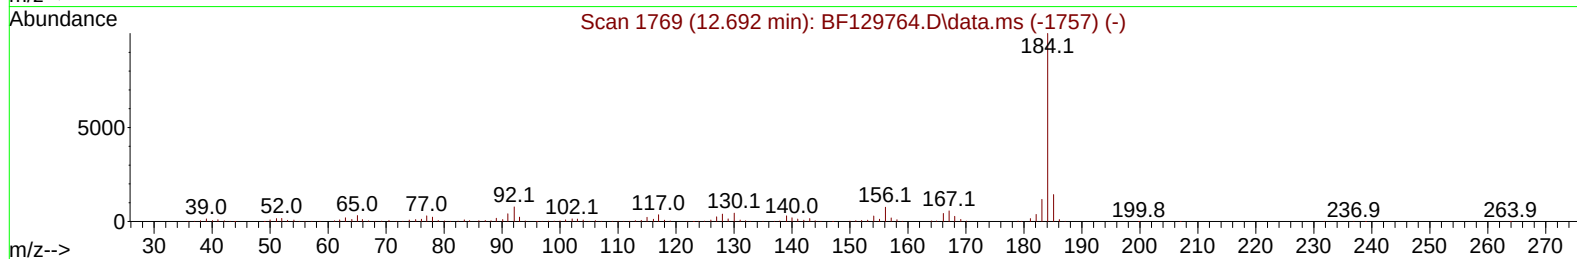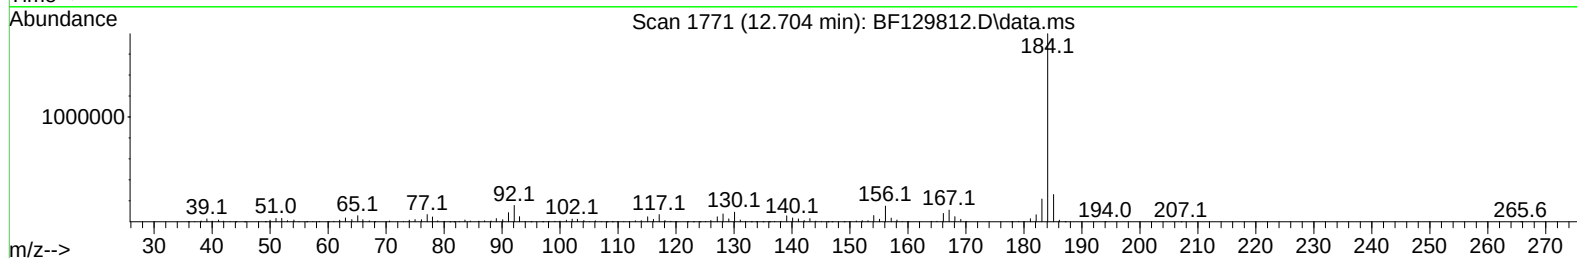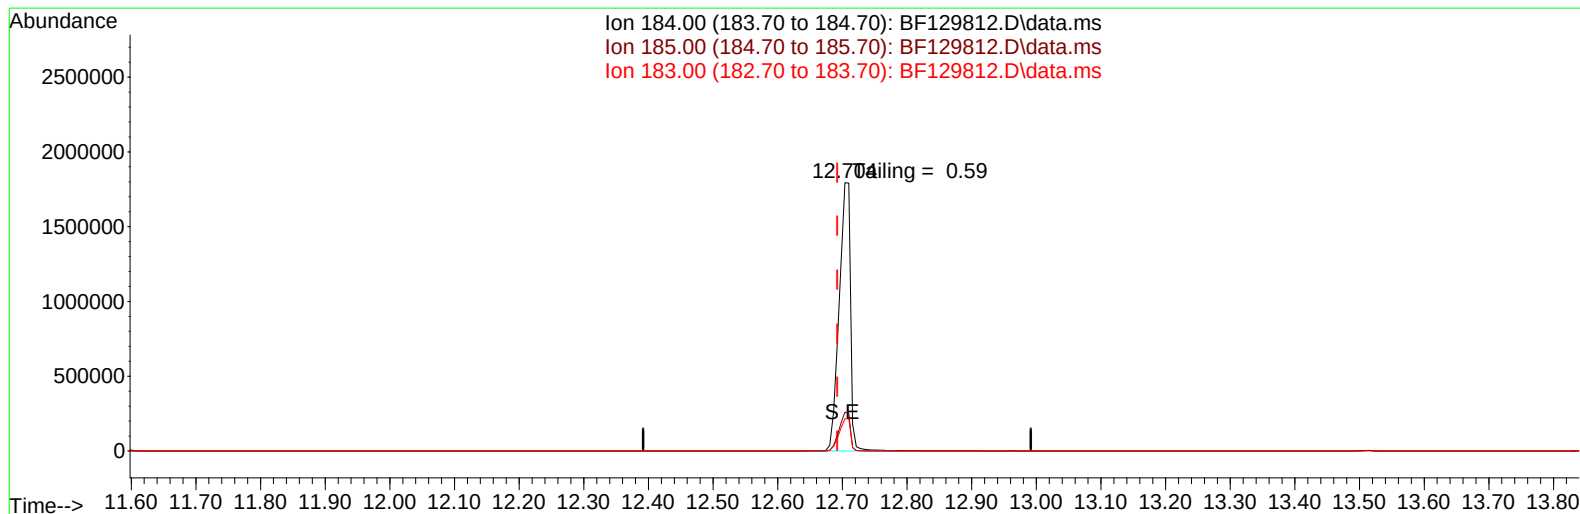

TIC: BF129812.D\data.ms

(77) Benzidine

12.704min (+ 0.012) 84522.76 ng

response 2184160

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.48
183.00	11.80	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/16/2022	BNA_F	<u>BF129812.D</u>
Compound Name	Response	Retention Time
DDT	1027327	13.516
DDD	9555	13.239
DDE	2224	12.874
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11779	1039106	1.13

Instrument :
BNA_F
ClientSampleId :
DFTPP