
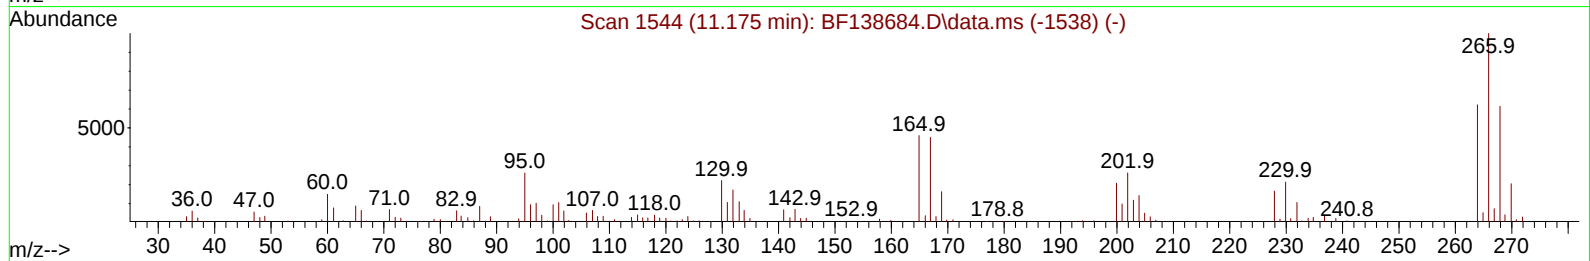
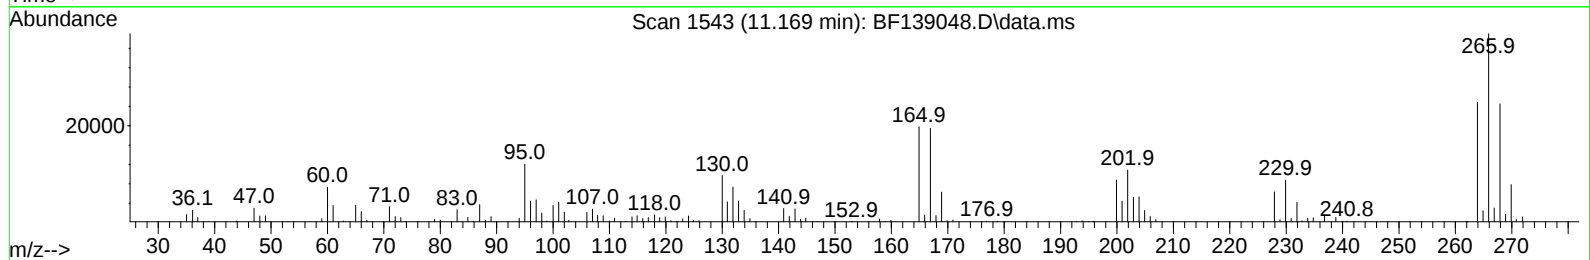


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081624\
Data File : BF139048.D
Acq On : 16 Aug 2024 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 12:21:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

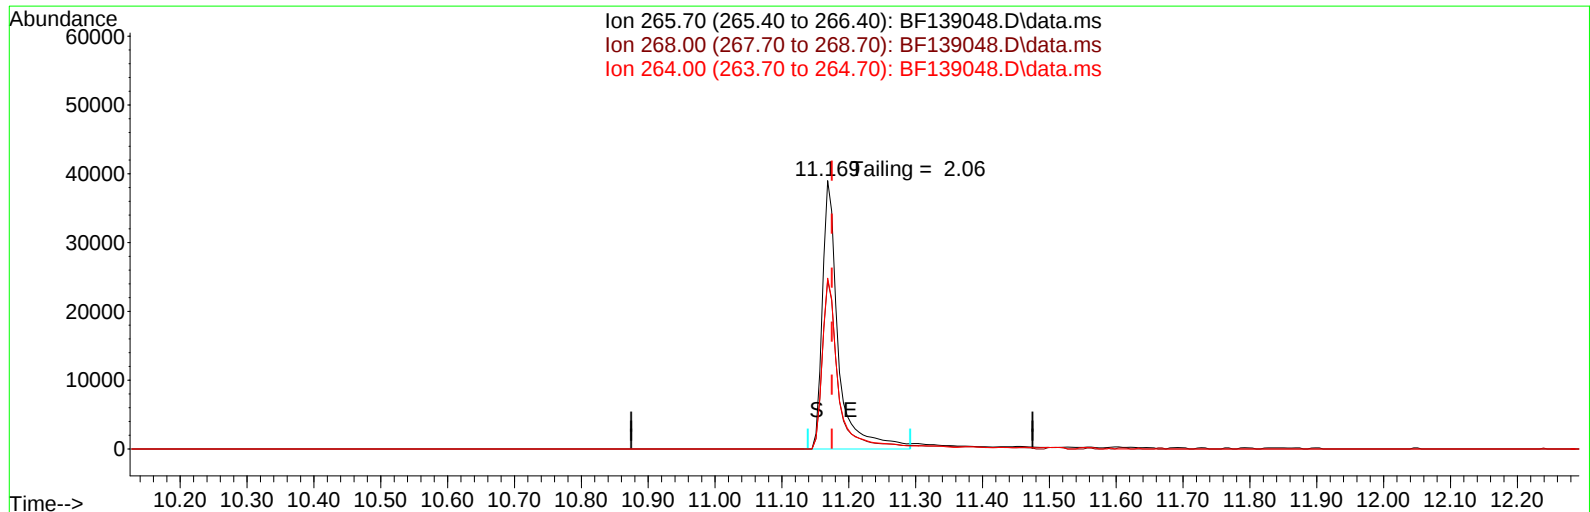

TIC: BF139048.D\data.ms

(70) Pentachlorophenol (C)




11.169min (-0.006) 38515.03 ng m

response 65013

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.90
264.00	62.20	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081624\
Data File : BF139048.D
Acq On : 16 Aug 2024 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 16 12:21:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

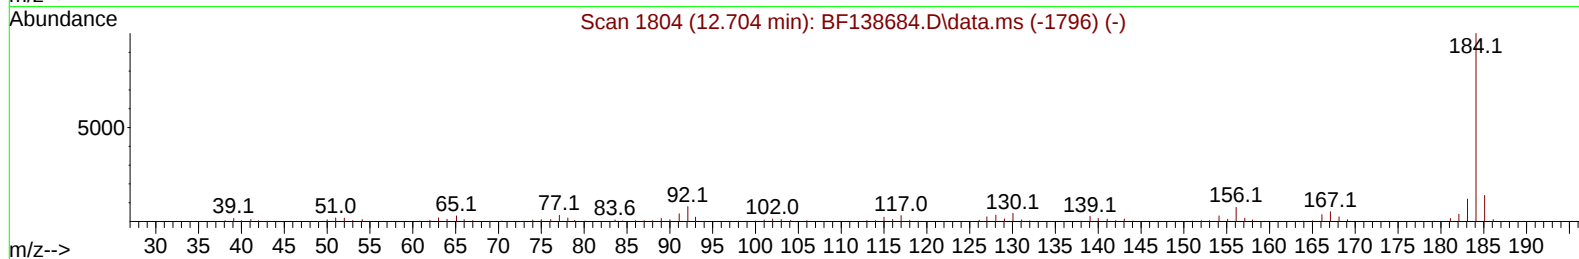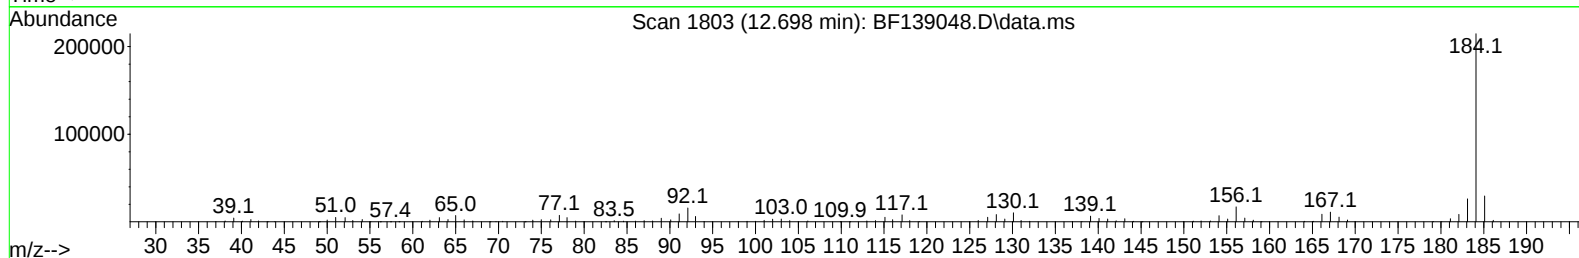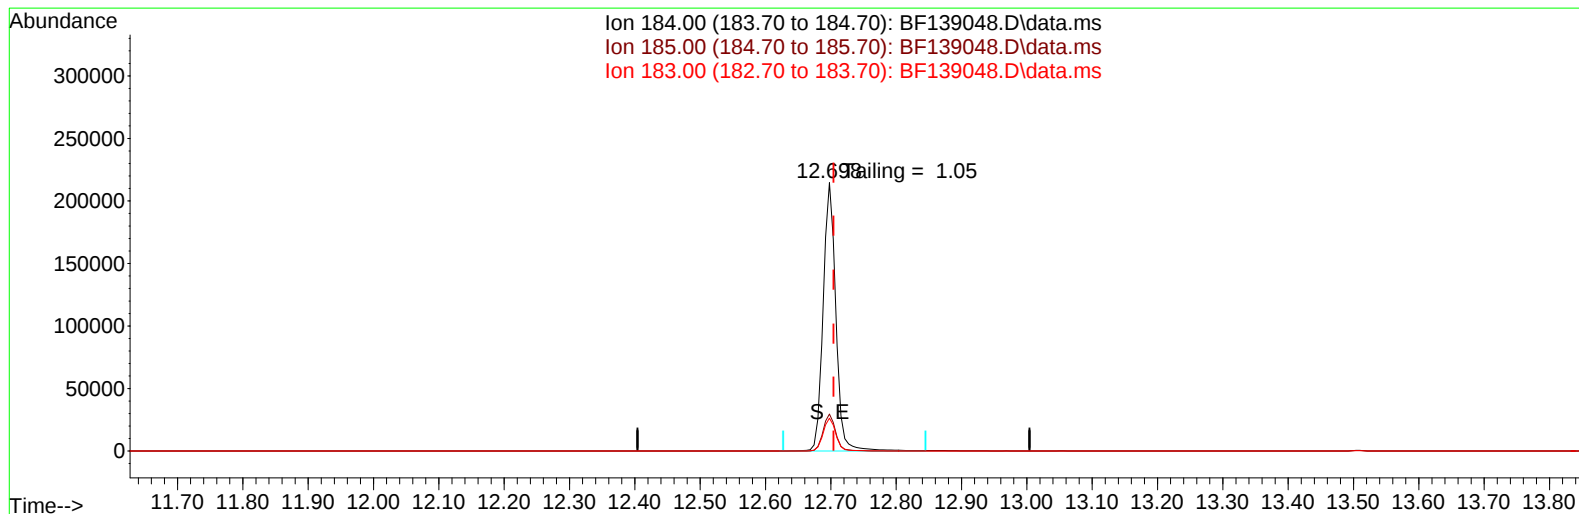

TIC: BF139048.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 291161

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.79
183.00	12.00	12.26
0.00	0.00	0.00