


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081624\
Data File : BF139048.D
Acq On : 16 Aug 2024 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

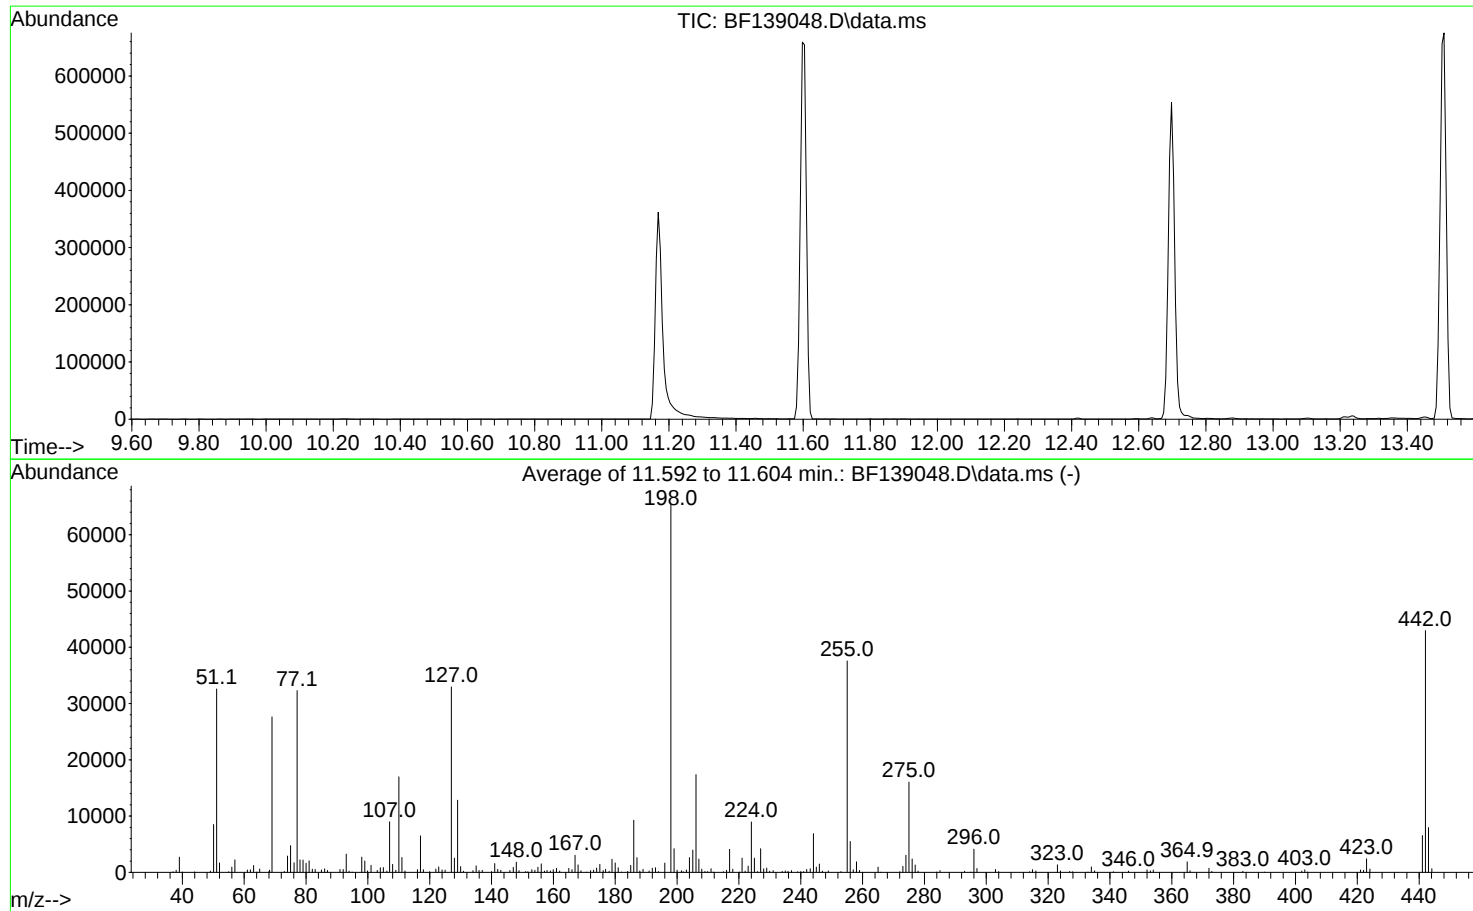

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	32595	PASS
68	69	0.00	2	1.4	400	PASS
69	198	0.00	100	42.3	27629	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	32957	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65371	PASS
199	198	5	9	6.5	4223	PASS
275	198	10	60	24.6	16050	PASS
365	198	1	100	2.9	1867	PASS
441	198	0.01	100	10.0	6550	PASS
442	442	50	100	100.0	42960	PASS
443	442	15	24	18.5	7962	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/16/2024	BNA_F	<u>BF139048.D</u>
Compound Name	Response	Retention Time
DDT	163291	13.51
DDD	3632	13.239
DDE	824	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4456	167747	2.66

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081624\
Data File : BF139048.D
Acq On : 16 Aug 2024 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 16 12:21:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

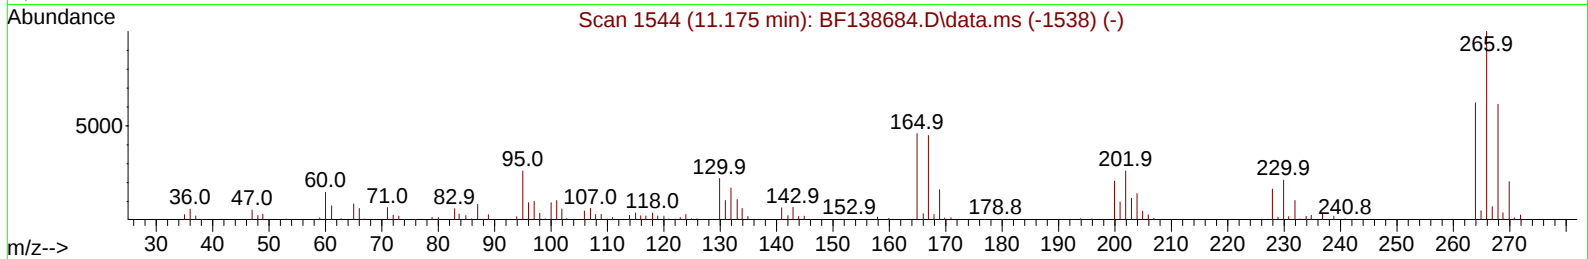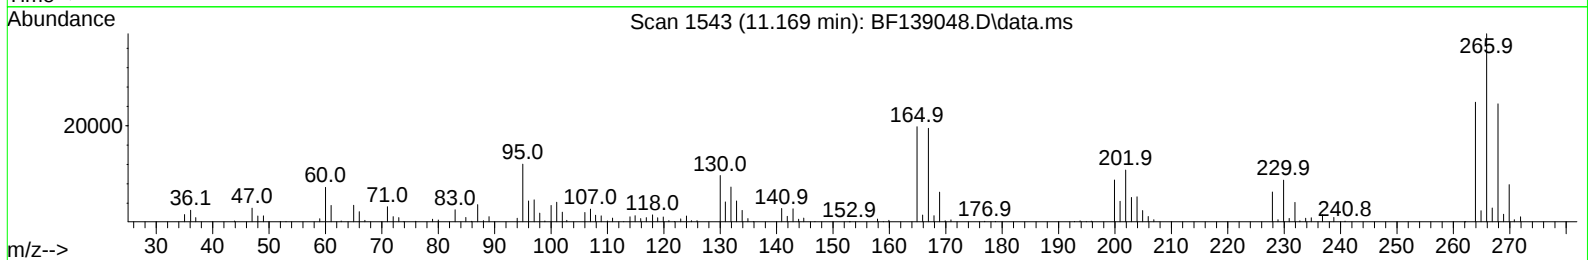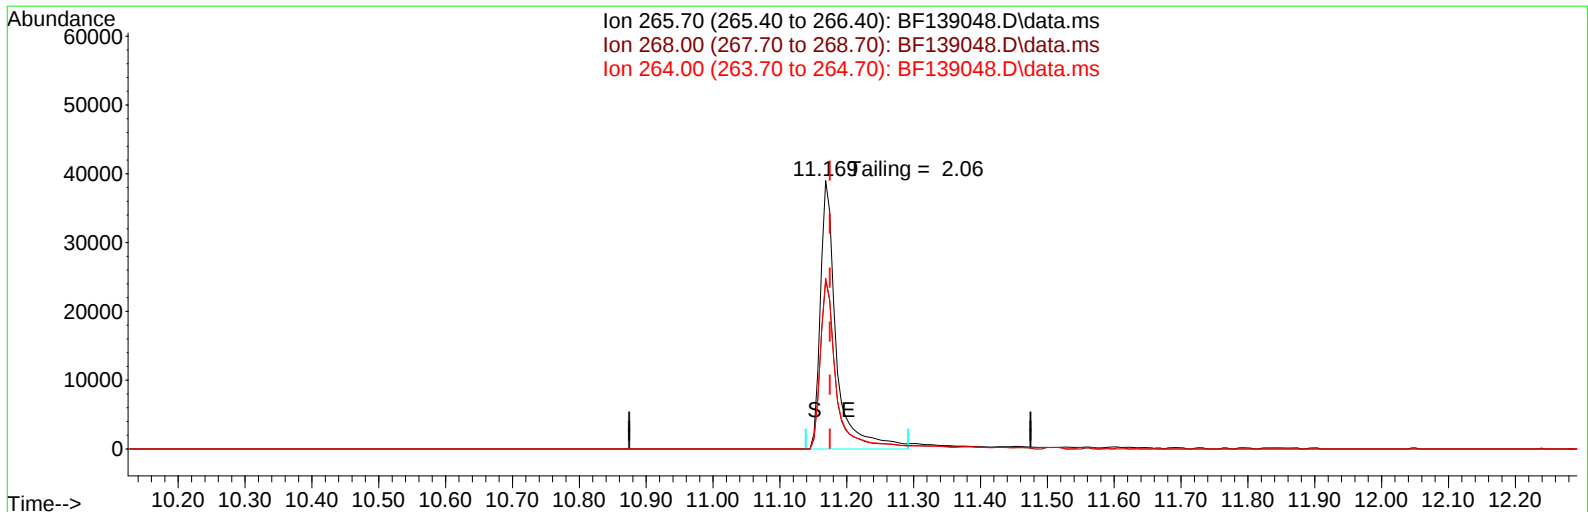

TIC: BF139048.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 38515.03 ng m




response 65013

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.90
264.00	62.20	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081624\
Data File : BF139048.D
Acq On : 16 Aug 2024 09:44
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 16 12:21:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

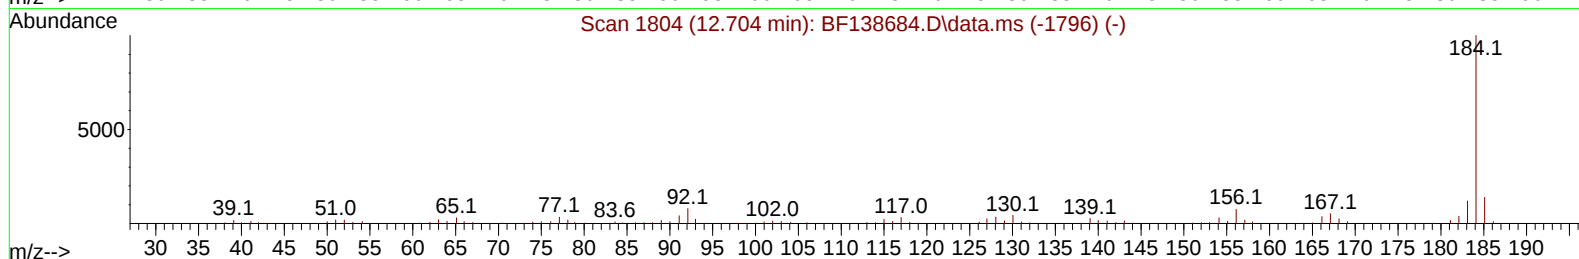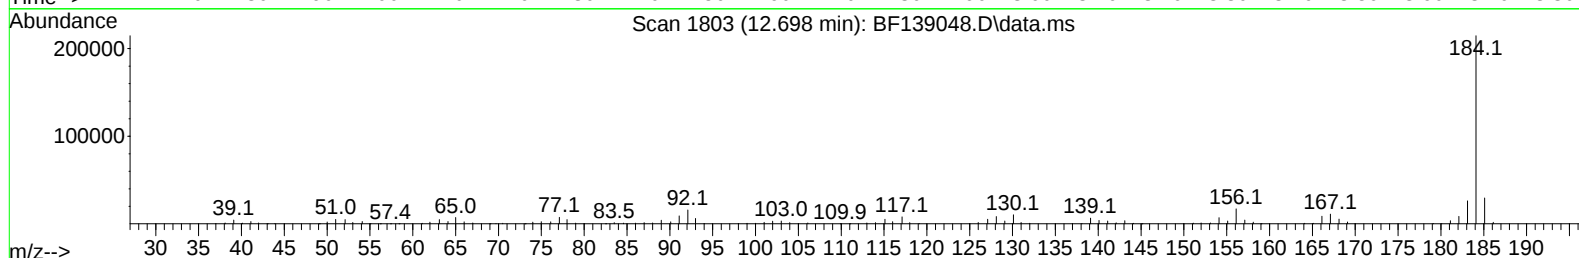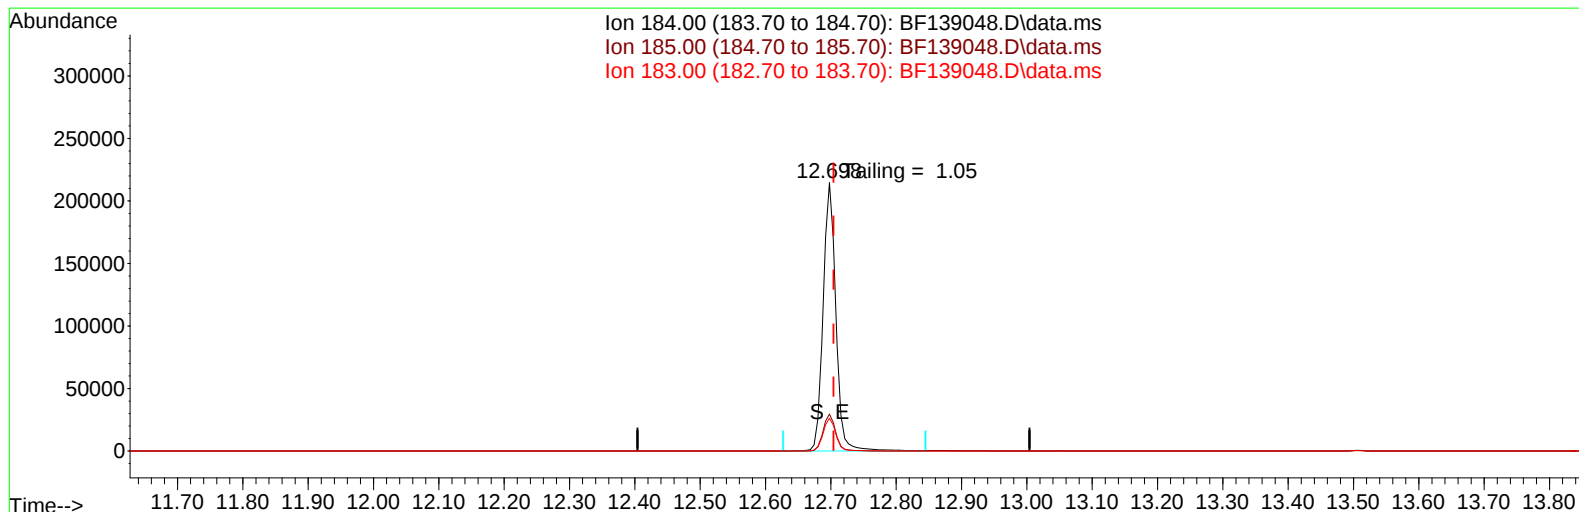

TIC: BF139048.D\data.ms

(77) Benzidine

12.698min (-0.006) 0.00 ng

response 291161

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.79
183.00	12.00	12.26
0.00	0.00	0.00